CNS-9701A
CNS-9701J
CNS-9701K

CENTRAL MONITOR

CNS-9701

0634-001842C

Model: CNS-9701

Manual code no.: 0634-001842C

Reader Comment Card

We welcome your comments about this manual. Your comments and suggestions help us improve our manuals. Please circle the number for each of the following statements corresponding to your evaluation and add comments in the space provided.

Fax or send your completed comment card to:
Fax: +81 (3) 5996-8100
International Div., Sales Promotion Section, Nihon Kohden Corp., 1-31-4, Nishiochiai Shinjuku-ku, Tokyo 161-8560, Japan

	Strongly Agree	Agree	Neutral	Disagree	Strongly Disagree
This manual is organized.	1	2	3	4	5
I can find the information I want.	1	2	3	4	5
The information is accurate.	1	2	3	4	5
I can understand the instructions.	1	2	3	4	5
The illustrations are appropriate and helpful.	1	2	3	4	5
The manual length is appropriate.	1	2	3	4	5

Comments:

Thank you for your cooperation. We appreciate it very much.

Name:
Occupation/Position:
Hospital/Company:
Address:

Phone:

cutting line

Contents

GENERAL HANDLING PRECAUTIONS i
WARRANTY POLICY ii
EMC RELATED CAUTION iii
Conventions Used in this Manual and Instrument v
Warnings, Cautions and Notes v
Explanations of the Symbols in this Manual and Instrument v

Section 1 General 1C.1

Introduction 1.1
General Information on Servicing 1.2
Service Policy, Service Parts and Patient Safety Checks 1.4
Service Policy 1.4
Service Parts 1.4
Maintenance Equipments and Tools 1.4
Important Safety Information 1.5
General 1.5
Installation 1.6
UPS 1.6
Network 1.7
Turning the Power On/Off 1.8
Discharge and Receiving Channel Change 1.8
Temporary Discharge 1.9
Patient Transfer 1.9
Alarm 1.9
ECG Monitoring 1.10
NIBP Measurement 1.10
Maintenance 1.11
Specification 1.12
Display 1.12
Waveform Display Items 1.12
Alphanumeric Display Items 1.12
Sound 1.12
Alarm Function 1.12
Trend 1.13
Waveform Sensitivity 1.13
Overview 1.13
Remote Setting 1.13
Full Disclosure 1.13
File Saving 1.13
2-ch recorder, WS-971R (option) 1.14
Laser Printer (local purchase) 1.14
Power Requirements 1.14
Environment 1.15
Electromagnetic Compatibility 1.15

Safety 1.15
Dimensions and Weight 1.15
Panel Descriptions 1.16
Central Monitor Main Unit MU-971RA/RJ/RK 1.16
Front Panel 1.16
Rear Panel 1.17
LCD Unit VL-971R/RK 1.18
Front 1.18
Rear 1.18
Recorder Unit WS-971R 1.19
Composition 1.20
Options 1.20
Connection Diagram 1.21

Section 2 Troubleshooting 2C.1

General 2.1
System 2.3
Network 2.4
Measurement Value 2.5
Alarm 2.5
Admitting/Discharging 2.6
All Beds Screen/Individual Bed Screen 2.7
Trend Window 2.8
Tabular Trend Window 2.8
Hemodynamics List Window 2.8
Arrhythmia Recall Window 2.9
ST Recall Window 2.9
Full Disclosure Window 2.10
ECG 12 Lead Analysis Window 2.10
Report Window 2.11
Recording 2.11
Overview Bed Screen 2.12
Parameter Setup 2.12
Power Problem 2.13
Display Problem 2.14
Touch Screen Problem 2.16
Sound Problem 2.16
Keyboard Problem 2.17
Mouse Problem 2.17
Hard Disk Problem 2.17
CD-ROM Drive or Floppy Disk Drive Problem 2.18
2-channel Recorder Unit Problem 2.18
Error Messages 2.19
Messages From Bedside Monitors/Multiple Patient Receiver 2.19
Messages about Measurement Conditions of Each Parameter 2.19
Other 2.24
Messages From Central Monitor 2.25
WS-971R Recorder Unit 2.25

Laser Printer 2.25
Other 2.25
Hard Disk Replacement Flow 2.26
How to Recover the BIOS Initial Settings 2.27
BIOS Default Setting (Vorax5000) 2.28
BIOS Default Setting (Vorax5001) 2.30

Section 3 Board/Unit Description 3C.1

Power Supply Unit (by NIPRON) 3.1
Motherboard (by A-OPEN) 3.1
CPU (1 GHz Pentium 3 or 2.4 GHz Pentium 4) Box 3.1
256 MB Memory DIMM S-DRAM or DDR266 ..... 3.2
40 GB Hard Disk (by IBM) 3.2
CD-ROM Drive (by SAMSUNG) 3.2
Graphic Board RADEON 32 or RADEON 7000 (by ATI) 3.2
PC Chassis IW-V500 or IW-V500G 3.3
Fan for Chassis 3.3
Mouse 3.3
RS232C Interface Board CYBER SERIAL 3.3

Section 4 Disassembly and Assembly 4C.1

Before You Begin 4.1
Warnings and Caution 4.1
Required Tools 4.1
Disassembling the Main Unit 4.2
Replacing the Motherboard 4.2
Replacing the Lithium Battery on the Motherboard 4.10
Replacing the CPU 4.10
Replacing the Internal Memory 4.10
Replacing the Hard Disk 4.11
Replacing the Graphic Board 4.11
Replacing the Fans 4.11
Replacing the Floppy Disk Drive 4.12
Replacing the Power Supply Unit 4.12
Replacing the CD Drive 4.12
Disassembling the Optional VL-971R Display Unit 4.13
Replacing the LCD Assembly 4.13
Removing the Display Unit Chassis 4.15
Replacing the Touch Screen 4.19
Disassembling the Optional WS-971R Recorder Unit 4.20
Removing the Recorder Sub Assy 4.20
Removing the AC Inlet Socket 4.21
Removing the RS232C Interface Board 4.22
Removing the Power Supply Unit 4.22
Removing the Front Panel 4.22
Replacing the LED 4.23
Replacing the Platen Roller/Bushings/Gear 4.24

Cleaning the Thermal Array Head/Paper Sensor 4.25
Operation Check after Assembling the Recorder Unit 4.25

Section 5 Maintenance 5C.1

To Be Replaced Periodically 5.1
Maintenance Check Items and Schedule 5.1
External and Connection 5.2
Display 5.2
Sound 5.2
Operation 5.3
Data Storage 5.3
Network Communication 5.4
Recorder 5.4
Laser Printer 5.4
UPS 5.5
Safety 5.5

Section 6 Adjustment 6C.1

Adjusting the VL-971R Display Unit 6.1
Automatic Adjustment 6.1
Manual Adjustment 6.2

Section 7 Replaceable Parts List 7C.1

MU-971RA/RJ/RK Main Unit (Vorax5000) 7.2
MU-971RA/RJ/RK Main Unit (Vorax5001) 7.4
VL-971R/RK Optional Display Unit 7.6
WS-971R Optional Recorder Unit 7.8

Section 8 Network Settings 8C.1

Network Setting Flowchart 8.2
Setting the IP Address on Each Instrument 8.3
Manually Setting the IP Address of the Central Monitor 8.3
Installing the Laser Printer (Network Printer) 8.6
Connecting the Network System 8.12
Start the System 8.12
Checking the Network Connection on the Central Monitor 8.13
Assigning the Group Name and Bed Name 8.14
Assigning a Bed Name/CNS Name 8.15
Assigning a CNS Name to a Central Monitor 8.15
Registering Group Names in the Central Monitor 8.15
Assigning a Group Name 8.16
Checking the Bed Name and Group Name Setting 8.16
Selecting the Monitored Beds 8.17
Changing Settings of System Setup, Patient Setting and Setup 8.19
Adding an Instrument to the Network During System Operation 8.20

Section 9 Connector Pin Assignment 9C.1

Sockets at the Rear of the Main Unit 9.1

SOUND Socket 9.1

TOUCH1/TOUCH2 Socket 9.1

VIDEO1/VIDEO2 Socket 9.2

RECORDER Socket 9.2

PROTECT KEY Socket 9.2

This page is intentionally left blank.

GENERAL HANDLING PRECAUTIONS

This device is intended for use only by qualified medical personnel.
Use only Nihon Kohden approved products with this device. Use of non-approved products or in a non-approved manner may affect the performance specifications of the device. This includes, but is not limited to, batteries, recording paper, pens, extension cables, electrode leads, input boxes and AC power.

Please read these precautions thoroughly before attempting to operate the instrument.

1. **To safely and effectively use the instrument, its operation must be fully understood.**

2. **When installing or storing the instrument, take the following precautions:**
   (1) Avoid moisture or contact with water, extreme atmospheric pressure, excessive humidity and temperatures, poorly ventilated areas, and dust, saline or sulphuric air.
   (2) Place the instrument on an even, level floor. Avoid vibration and mechanical shock, even during transport.
   (3) Avoid placing in an area where chemicals are stored or where there is danger of gas leakage.
   (4) The power line source to be applied to the instrument must correspond in frequency and voltage to product specifications, and have sufficient current capacity.
   (5) Choose a room where a proper grounding facility is available.

3. **Before Operation**
   (1) Check that the instrument is in perfect operating order.
   (2) Check that the instrument is grounded properly.
   (3) Check that all cords are connected properly.
   (4) Pay extra attention when the instrument is in combination with other instruments to avoid misdiagnosis or other problems.
   (5) All circuitry used for direct patient connection must be doubly checked.
   (6) Check that battery level is acceptable and battery condition is good when using battery-operated models.

4. **During Operation**
   (1) Both the instrument and the patient must receive continual, careful attention.
   (2) Turn power off or remove electrodes and/or transducers when necessary to assure the patient's safety.
   (3) Avoid direct contact between the instrument housing and the patient.

5. **To Shutdown After Use**
   (1) Turn power off with all controls returned to their original positions.
   (2) Remove the cords gently; do not use force to remove them.
   (3) Clean the instrument together with all accessories for their next use.

6. **The instrument must receive expert, professional attention for maintenance and repairs. When the instrument is not functioning properly, it should be clearly marked to avoid operation while it is out of order.**

7. **The instrument must not be altered or modified in any way.**

8. **Maintenance and Inspection:**
   (1) The instrument and parts must undergo regular maintenance inspection at least every 6 months.
   (2) If stored for extended periods without being used, make sure prior to operation that the instrument is in perfect operating condition.

(3) Technical information such as parts list, descriptions, calibration instructions or other information is available for qualified user technical personnel upon request from your Nihon Kohden distributor.

9. **When the instrument is used with an electrosurgical instrument, pay careful attention to the application and/or location of electrodes and/or transducers to avoid possible burn to the patient.**

10. **When the instrument is used with a defibrillator, make sure that the instrument is protected against defibrillator discharge. If not, remove patient cables and/or transducers from the instrument to avoid possible damage.**

WARRANTY POLICY

Nihon Kohden Corporation (NKC) shall warrant its products against all defects in materials and workmanship for one year from the date of delivery. However, consumable materials such as recording paper, ink, stylus and battery are excluded from the warranty.

NKC or its authorized agents will repair or replace any products which prove to be defective during the warranty period, provided these products are used as prescribed by the operating instructions given in the operator's and service manuals.

No other party is authorized to make any warranty or assume liability for NKC's products. NKC will not recognize any other warranty, either implied or in writing. In addition, service, technical modification or any other product change performed by someone other than NKC or its authorized agents without prior consent of NKC may be cause for voiding this warranty.

Defective products or parts must be returned to NKC or its authorized agents, along with an explanation of the failure. Shipping costs must be pre-paid.

This warranty does not apply to products that have been modified, disassembled, reinstalled or repaired without Nihon Kohden approval or which have been subjected to neglect or accident, damage due to accident, fire, lightning, vandalism, water or other casualty, improper installation or application, or on which the original identification marks have been removed.

In the USA and Canada other warranty policies may apply.

CAUTION

United States law restricts this device to sale by or on the order of a physician.

EMC RELATED CAUTION

This equipment and/or system complies with the International Standard IEC 60601-1-2 for electromagnetic compatibility for medical electrical equipment and/or system. However, an electromagnetic environment that exceeds the limits or levels stipulated in the IEC 60601-1-2, can cause harmful interference to the equipment and/or system or cause the equipment and/or system to fail to perform its intended function or degrade its intended performance. Therefore, during the operation of the equipment and/or system, if there is any undesired deviation from its intended operational performance, you must avoid, identify and resolve the adverse electromagnetic effect before continuing to use the equipment and/or system.

The following describes some common interference sources and remedial actions:

1. **Strong electromagnetic interference from a nearby emitter source such as an authorized radio station or cellular phone:**
   Install the equipment and/or system at another location if it is interfered with by an emitter source such as an authorized radio station. Keep the emitter source such as cellular phone away from the equipment and/or system.

2. **Radio-frequency interference from other equipment through the AC power supply of the equipment and/or system:**
   Identify the cause of this interference and if possible remove this interference source. If this is not possible, use a different power supply.

3. **Effect of direct or indirect electrostatic discharge:**
   Make sure all users and patients in contact with the equipment and/or system are free from direct or indirect electrostatic energy before using it.

4. **Electromagnetic interference with any radio wave receiver such as radio or television:**
   If the equipment and/or system interferes with any radio wave receiver, locate the equipment and/or system as far as possible from the radio wave receiver.

If the above suggested remedial actions do not solve the problem, consult your Nihon Kohden Corporation subsidiary or distributor for additional suggestions.

The CE mark is a protected conformity mark of the European Community. The products herewith comply with the requirements of the Medical Device Directive 93/42/EEC.

The CE mark only applies to the CNS-9701K series central monitors.

This equipment complies with EUROPEAN STANDARD EN-60601-1-2 (1993) which requires EN-55011, class A. Class A EQUIPMENT is allowed in domestic establishments when used under the jurisdiction of a health care professional.

In IEC 60601-1-2 Medical Electronic Equipment, Part 1: General Requirements for Safety, 2. Collateral Standard: Electromagnetic compatibility-Requirements and test. Section 36. 202. 2 Radiated radio-frequency electromagnetic fields, PATIENT COUPLED EQUIPMENT and/or SYSTEMS applicable IMMUNITY test methods are under consideration at SC62A/WG13. The 3 V/m IMMUNITY level may be inappropriate especially when measuring SpO_2 because physiological signals can be much smaller than those induced by a 3 V/m electromagnetic field.

When measuring SpO_2, various interference may produce false waveforms which look like pulse waveforms. SpO_2 value and pulse rate may be measured from these false waveforms, causing the alarm to function improperly.

When installing the monitor, avoid locations where the monitor may receive strong electromagnetic interference such as radio or TV stations, cellular phone or mobile two-way radios.

Conventions Used in this Manual and Instrument

Warnings, Cautions and Notes

Warnings, cautions and notes are used in this manual to alert or signal the reader to specific information.

WARNING

A warning alerts the user to possible injury or death associated with the use or misuse of the instrument.

CAUTION

A caution alerts the user to possible injury or problems with the instrument associated with its use or misuse such as instrument malfunction, instrument failure, damage to the instrument, or damage to other property.

NOTE

A note provides specific information, in the form of recommendations, prerequirements, alternative methods or supplemental information.

Explanations of the Symbols in this Manual and Instrument

The following symbols found in this manual/instrument bear the respective descriptions as given.

On MU-971RA/RJ/RK central monitor main unit

Symbol	Description	Symbol	Description
	Power ON		Hard disk lamp
	Power OFF		Reset
	Attention, consult operator's manual		Mouse socket
	System start/shutdown		Keyboard socket
	Power lamp (Power ON)		(Only for CNS-9701K) The CE mark is a protected conformity mark of the European Community. The products herewith comply with the requirements of the Medical Device Directive 93/42/EEC.

On Screen

Symbol	Description	Symbol	Description
	Overview		Adjust setting/Scroll data
	Help		Alarm
	Print Stop		Speaker
	Delayed recording start		Electrocardiogram
	Print mark/Print		Alarm suspend/silence with remaining minutes at the central monitor
	Menu (System Setup)		Alarm suspend at the transmitter
	Previous		All alarm off, vital sign alarm off
	All Beds		Alarm recording off
	Deletion mark		QRS sync mark
	Close a window		

On VL-971R/RK LCD unit

Symbol	Description	Symbol	Description
	Power on		Attention, consult operator's manual
	Power off		

On WS-971R Recorder Unit

Symbol	Description	Symbol	Description
	Power on		Fuse
	Power off		Type B applied part

For the symbol marks on the locally purchaced LCD display, laser printer and UPS, refer to each instruction manual.

Section 1 General

Introduction 1.1
General Information on Servicing 1.2
Service Policy, Service Parts and Patient Safety Checks 1.4
- Service Policy 1.4
- Service Parts 1.4
- Maintenance Equipments and Tools 1.4

Important Safety Information 1.5
- General 1.5
- Installation 1.6
- UPS 1.6
- Network 1.7
- Turning the Power On/Off 1.8
- Discharge and Receiving Channel Change 1.8
- Temporary Discharge 1.9
- Patient Transfer 1.9
- Alarm 1.9
- ECG Monitoring 1.10
- NIBP Measurement 1.10
- Maintenance 1.11

Specification 1.12
- Display 1.12
- Waveform Display Items 1.12
- Alphanumeric Display Items 1.12
- Sound 1.12
- Alarm Function 1.12
- Trend 1.13
- Waveform Sensitivity 1.13
- Overview 1.13
- Remote Setting 1.13
- Full Disclosure 1.13
- File Saving 1.13
- 2-ch recorder, WS-971R (option) 1.14
- Laser Printer (local purchase) 1.14
- Power Requirements 1.14

Environment 1.15
Electromagnetic Compatibility 1.15
Safety 1.15
Dimensions and Weight 1.15
Panel Descriptions 1.16
Central Monitor Main Unit MU-971RA/RJ/RK 1.16
Front Panel 1.16
Rear Panel 1.17
LCD Unit VL-971R/RK 1.18
Front 1.18
Rear 1.18
Recorder Unit WS-971R 1.19
Composition 1.20
Options 1.20
Connection Diagram 1.21

Introduction

This service manual provides useful information to qualified service personnel to understand, troubleshoot, service, maintain and repair the CNS-9701A/J/K Central Monitor (referred to as “monitor” in this service manual).

All replaceable parts or units of this monitor and its optional units are clearly listed to help you locate the parts quickly.

The “Maintenance” section in this service manual only describes the maintenance that should be performed by qualified service personnel. The Maintenance section in the operator’s manual describes the maintenance that can be performed by the user.

The information in the operator’s manual is primarily for the user. However, it is important for service personnel to thoroughly read the operator’s manual and service manual before starting to troubleshoot, service, maintain or repair this monitor. This is because service personnel need to understand the operation of the monitor in order to effectively use the information in the service manual.

General Information on Servicing

Note the following information when servicing the monitor.

WARNING

To avoid the possibility of injury to yourself or damage to the monitor, do not install or remove any component while the power is on. When disassembling, make sure that the monitor is turned off and the power cord is disconnected from the monitor and AC outlet. There is a high voltage circuit on the power unit.

CAUTIONS

Safety

- **There is the possibility that the outside surface of the monitor, such as the operation keys, could be contaminated by contagious germs so disinfect and clean the monitor before servicing it. When servicing the monitor, wear rubber gloves to protect yourself from infection.**

- **There is the possibility that when the lithium battery or LCD unit is broken, a solvent could flow out or a toxic substance inside it could come out. If the solvent or toxic substance contacts the eyes or skin, wash immediately and thoroughly with water and see your physician. Never rub your eyes, otherwise you may lose your eyesight.**

- **To avoid accidental electrostatic discharge which could damage the components of the monitor, use a grounded wrist strap when installing or removing any component of the monitor.**

- **Use a pair of clean cotton gloves when replacing the LCD unit. If it is damaged, your hand may get injured.**

Liquid ingress

The monitor is not waterproof, so do not install the monitor where water or liquid can get into or fall on the monitor. If liquid accidentally gets into the monitor or the monitor accidentally falls into liquid, disassemble the monitor, clean it with clean water and dry it completely. After reassembling, do the patient safety checks and function/performance checks to verify that there is nothing wrong. If there is something wrong with the monitor, contact your Nihon Kohden representative for repair.

Environmental Safeguards

Depending on the local laws in your community, it may be illegal to dispose of the lithium battery in the regular waste collection. Check with your local officials for proper disposal procedures.

Disinfection and cleaning

To disinfect the outside surface of the monitor, wipe it with a non-abrasive cloth moistened with any of the disinfectants listed below. Do not use any other disinfectants or ultraviolet rays to disinfect the monitor.

- **Chlorohexidine gluconate solution: 0.5%**
- **Benzethonium chloride solution: 0.2%**
- **Glutaraldehyde solution: 2.0%**
- **Benzalkonium chloride: 0.2%**
- **Hydrochloric alkyl diaminoethylglycine: 0.5%**

Transport

- **Use the specified shipment container and packing material to transport the monitor. If necessary, double pack the monitor. Also, put the monitor into the shipment container after packing so that the buffer material does not get inside the monitor.**
- **When transporting a board or unit of the monitor, be sure to put it in a conductive bag. Never use an aluminum bag to transport a board or unit. Also, never use a styrene foam or plastic bag which generates static electricity to wrap the board or unit of the monitor.**

Handling the monitor

- **Because the outside surface of the monitor is made of resin, the outside surface of the monitor is easily damaged. So when handling the monitor, remove clutter from around the monitor and be careful to not damage the monitor or get it dirty.**
- **Because most of the boards in the monitor are multilayer boards with surface mount electrical devices (SMD), a special tool is required to remove and solder the electrical devices on it. To avoid damaging other electrical components, do not remove and solder SMD components yourself.**

Measuring and Test Equipment

Maintain the accuracy of the measuring and test equipment by checking and calibrating it according to the check and calibration procedures.

Lithium Battery

- **Before disposing of the battery, check with your local solid waste officials for details in your area for recycling options or proper disposal. The battery is recyclable. At the end of its useful life, under various state and local laws, it may be illegal to dispose of this battery into the municipal waste stream.**

Service Policy, Service Parts and Patient Safety Checks

Service Policy

Our technical service policy for this monitor is to replace the faulty unit, board or part or damaged mechanical part with a new one. Do not perform electrical device or component level repair of the multilayer board or unit. We do not support component level repair outside the factory for the following reasons:

- Most of the boards are multilayer boards with surface mount electrical devices, so the mounting density of the board is too high.
- A special tool or high degree of repair skill is required to repair the multilayer boards with surface mount electrical devices.

Only disassemble the monitor or replace a board or unit in an environment where the monitor is protected against static electricity.

As background knowledge for repair, pay special attention to the following:

- To reduce the repair time, consider the problem before starting repair.
- To clarify the source of the troubles, use the information from the diagnostic check function of the monitor and the information described in the troubleshooting section.

Service Parts

Refer to "Replaceable Parts List" of this manual for the service parts for technical service that we provide.

NOTE

When ordering parts or accessories from your Nihon Kohden representative, please quote the NK code number and part name which is listed in this service manual, and the name or model of the unit in which the required part is located. This will help us to promptly attend to your needs. Always use parts and accessories recommended or supplied by Nihon Kohden Corporation to assure maximum performance from your monitor.

Maintenance Equipments and Tools

Test equipment

When repairing or calibrating the monitor, the following test equipment is required.

- Digital voltmeter: standard type (An oscilloscope can be used instead of the digital voltmeter.)

Important Safety Information

General

WARNING

- **Never use the central monitor in the presence of any flammable anesthetic gas, concentrated oxygen or hyperbaric oxygen. Failure to follow this warning may result in explosion.**
- **Never use the central monitor in a high-pressure oxygen medical care tank. Failure to follow this warning may cause explosion or fire.**
- **Do not install any software other than specified by Nihon Kohden and run it in the central monitor. Otherwise Nihon Kohden does not warrant normal operation of the CNS-9701 system program.**
- **Do not install the CNS-9701 system software into a personal computer which is not specified by Nihon Kohden and use it for monitoring.**
  - **If the personal computer does not satisfy the performance specifications which are required by Nihon Kohden, the system software may not function normally.**
  - **If the personal computer does not satisfy the safety standards which are required by Nihon Kohden, the patient and operator may get electrical shock through another instrument in the network.**
- **While the central monitor is on, do not insert any CD-ROM or floppy disk into it. Nihon Kohden does not warrant the normal operation of the central monitor in the case that an application or software installation starts automatically.**

CAUTION

- **If any liquid might have gotten into the central monitor, take it out of service and contact your Nihon Kohden distributor or representatives.**
- **While the central monitor is on, do not touch unused sockets. Failure to follow this caution may damage the monitor by static electricity and may cause malfunction.**

Installation

WARNING

Install the central monitor and external instruments outside the patient environment (IEC 60601-1-1 2.204). If they are installed inside the patient environment, the patient or operator may receive electrical shock. For installation, contact your Nihon Kohden distributor or representative.

CAUTION

- **Only use the provided power cord. Using other power cords may result in electrical shock or other injury to the patient and operator.**
- **Before connecting or disconnecting instruments, turn each instrument off and disconnect each power cord from the AC socket. Failure to follow this caution may cause electrical shock.**
- **Connect only the specified instruments to the central monitor by following the specified procedure. Otherwise, electrical leakage current may harm the patient and operator.**
- **Do not let connection cables stick out; run them along the floor or wall. If people trip over the cable, the monitor may tip over and it may cause injury.**

UPS

WARNING

- **Install the UPS outside the patient environment (IEC 60601-1-1 2.204). If it is installed inside the patient environment, the safety standards which are required by Nihon Kohden are not satisfied and it may cause electrical shock to the patient or operator.**
- **Use a UPS which satisfies the safety standards specified by IEC and UL. Otherwise, lack of safety may cause electrical shock to the patient or operator.**
- **Periodically check the life of the UPS battery. Replace the battery when the lifetime expires. If the battery is used beyond its lifetime, liquid leakage, smoke, fire or explosion may occur.**

CAUTION

- **Make sure that the UPS is properly grounded. Otherwise the operator may receive electrical shock.**
- **To assure an uninterrupted power supply, we recommend using the specified UPS. A sudden loss of power supply or an extreme power surge can damage the central monitor and delete stored data.**

Network

WARNING

- **Connect the central monitor to the network as specified in the Network and System Installation Guide. Otherwise the patient and operator may get electrical shock or other injury. For connecting the network, contact your Nihon Kohden distributor or representatives.**
- **Check the software version number of the monitor before connecting it to the network. Different software versions have different communication methods. When there is more than one communication method in the network, communication may malfunction.**
- **Install the external instruments including the printer and hubs outside the patient environment (IEC 60601-1-1 2.204). If they are installed inside the patient environment, the patient or operator may receive electrical shock. For installation, contact your Nihon Kohden distributor or representatives.**

CAUTION

- **Network settings and Windows 2000 system settings must only be set by a qualified service personnel. Contact your Nihon Kohden distributor or representatives.**
- **The network must be managed by the network administrator. Make sure that each monitor in the network has a different IP address. Otherwise, data communication cannot be performed properly and it causes incorrect monitoring. When adding a monitor to an already operating network, set the IP address on the monitor before connecting the monitor to the network.**

Turning the Power On/Off

WARNING

- **Do not turn off the display to which the sound cable is connected. Otherwise there is no alarm sound.**
- **Do not adjust the sound volume at the display unit. If you decrease the display unit volume to the minimum, there is no alarm sound.**
- **When monitoring with two displays, do not turn off either display. Otherwise some monitored beds cannot be monitored.**

CAUTION

- **Follow the specified procedure to turn off the central monitor. Otherwise, patient data will be deleted and data in the hard disk and the hard disk itself may be damaged.**
- **After turning the power on, confirm that there is a test sound from the built-in speaker of the display.**

Discharge and Receiving Channel Change

WARNING

- **Check that the channel number of the appropriate transmitter is displayed on the central monitor screen. Otherwise data of a different patient will be monitored or no signal will be received by the central monitor.**
- **Do not use the same channel for different patients. Otherwise two patients' data will be lost due to mutual modulation interference or another patient's data may appear on the monitor screen.**

CAUTION

- **When admitting a new patient, first delete all data of the previous patient. Otherwise, the data of the previous patient and new patient will be mixed together and cause misunderstanding of the patient history.**
- **When you change the receiving channel to monitor a new patient, first delete all data of the previous patient. Otherwise, the data of the previous patient and new patient will be mixed together and cause misunderstanding of the patient history.**

Temporary Discharge

WARNING

When a temporarily discharged patient comes back, resume monitoring for the patient. During temporary discharge, there is no display of measurement values, alarm function and data saving.

Patient Transfer

CAUTION

- **Keep the original bedside monitor and the destination bedside monitor power on and connected to the network until the transfer completes. Otherwise transfer fails and the data is lost. After transfer, confirm that the data was correctly transferred to the destination bedside monitor.**
- **When the patient is transferred more than once between different central monitors in the network, the data saved on the original central monitor is deleted.**

Alarm

WARNING

- **When the Alarm Suspend key on the transmitter is pressed, all alarm functions for the patient are suspended.**
- **Even if the alarm is set to ON, there is no arrhythmia alarm when arrhythmia analysis is turned OFF at the bedside monitor and/or central monitor.**
- **Before you start monitoring a new patient, confirm alarm settings. Alarm settings return to Alarm Master 1 settings when a bed is discharged or a receiving channel is changed.**
- **Securely connect the sound cable. There is no sound if the cable comes off.**

CAUTION

- **When the upper or lower alarm limit is set to OFF, there will be no upper or lower alarm for that limit. When it is set to OFF, frequently observe the patient.**
- **Alarm does not occur for an arrhythmia whose alarm is set to OFF. There is no indication that the alarm is set to OFF. Be careful when you set the alarm to OFF.**

ECG Monitoring

CAUTION

- **If there is any doubt about the arrhythmia analysis, make the central monitor relearn the patient's VPC. Otherwise, an important arrhythmia may be overlooked.**
- **The central monitor does not perform ECG analysis. Therefore, the QRS sound at the central monitor may not synchronize with patient's actual QRS when complicated arrhythmias occur or during pacing.**
- **The ST level transmitted from a transmitter is not designed to be accurate enough for diagnosis. Do not rely on the ST level displayed on the central monitor.**
- **The QRS sound at the central monitor has a delay of approximately several seconds because of network connection.**
- **When the full disclosure waveform is expanded to actual size, it may be distorted because it has been compressed then expanded. When reading the expanded ECG waveforms, be aware of this distortion.**
- **Turn the pacing detection to ON when monitoring a pacemaker patient. Otherwise QRS and pacemaker spike may not be distinguished and pacemaker failure may not be recognized.**

NIBP Measurement

WARNING

- **When performing long term measurements at intervals less than 2.5 minutes, periodically check the state of the patient, blood vessels and limb for adequate circulation. Congestion may occur at the measurement site.**
- **When performing periodic measurements for a long term, periodically check the circulation condition.**

CAUTION

Before you remotely start and stop NIBP measurement from the central monitor, confirm the state of the patient at the bedside monitor. Carefully start and stop NIBP measurement from the central monitor.

Maintenance

CAUTION

- **Before maintenance (inspection, cleaning, disinfection), turn the central monitor power off and disconnect the power cord from the AC outlet. Otherwise the operator may receive electrical shock or the central monitor may malfunction.**
- **Do not disassemble or repair the central monitor. Disassembly and repair must be performed by qualified service personnel.**
- **Software upgrade must only be done by qualified service personnel or a person with technical knowledge. If upgrade is not done correctly, the central monitor may freeze.**
- **Do the regular inspection according to the cycle specified by Nihon Kohden. Otherwise, deterioration and loss of function are overlooked and it results in incorrect monitoring.**
- **Restart the central monitor once every three months. Otherwise the operation becomes unstable and monitoring may stop. During restarting, patients monitored by the central monitor must be monitored by another instrument.**
- **Replace the hard disk once every two years. If the hard disk gets damaged, monitoring is incorrect and all data saved in the central monitor is lost.**

For the VL-971R/RK LCD unit

- **Follow your hospital regulations to handle blood or bodily fluids on the display.**
- **Be careful not to let any liquid get inside the display.**

Specification

Display

Number of patients on the display	16 patients max With overview bed function, 16 patients plus one other patient.
Number of transmitters	16 transmitters max
Display type	18 inch color TFT
Waveform display method	Non-fade, fixed method
Number of waveform traces	Single display: 24 traces max (On the All Beds screen, displaying 12 patients) Dual display: 32 traces max (On the All Beds screen, displaying 16 patients)
Sweep speed	25 mm/s, 50 mm/s, 6.25 mm/s (respiration measurement)
Sweep time	All Beds screen (8 patients): 4.48 s All Beds screen (4 patients): 11.56 s Individual Bed screen: 10.28 s

Waveform Display Items

ECG1 - 12, IBP (1- 8), respiration wave, EEG, CO_2, external input, pulse (SpO_2), Flow/Paw, anesthetic gas (O_2, CO_2, N_2O, Agent), others depending on the connected bedside monitor or transmitter

Alphanumeric Display Items

Heart rate, VPC rate, respiration rate, pulse rate, IBP (systolic, diastolic, mean), NIBP (systolic, diastolic, mean), temperature or ΔT or blood temperature, $EtCO_2$, $tcPO_2$, $tcPCO_2$, SpO_2, ST level, FiO_2, CO, CCO, respirator, anesthetic gas, BIS, $S\bar{v}O_2$, Flow/Paw, N_2O, O_2, agent, others depending on the connected bedside monitor or transmitter

Sound

Synchronization source	ECG
Alarm sound	Crisis, Warning, Advisory
Sound volume	changeable for Heart rate sync mark and sound

Alarm Function

Alarm decision is done at each bedside monitor and multiple patient receiver. The central monitor only displays the alarm and generates sound by receiving the alarm information from bedside monitors and multiple patient receivers.

Alarm type	Crisis, Warning, Advisory	
Alarm items	Vital Sign:	Heart rate, VPC rate, Respiration rate, Pulse rate, ST level, BP (sys, dia, mean), NIBP (sys, dia, mean), temperature or ΔT or blood temperature, $EtCO_2$, $tcPO_2$, $tcPCO_2$, SpO_2, FiO_2, CCO, others depending on the connected bedside monitor or transmitter

	Arrhythmia:	ASYSTOLE, V FIB, V TACHY, EXT TACHY, EXT BRADY, VPC RUN, COUPLET, MULTI FORM, EARLY VPC, BIGEMINY, TACHY, BRADY, PROLONGED RR, FREQ. VPC
	Apnea	
Alarm display	Highlighted numeric display, highlighted message for arrhythmia	
Alarm occurrence	Alarm occurs when any one of the bedside monitors that the central monitor are monitoring generates alarm.	
Alarm suspend	Available (for beds connected via the QI-910R interface)	
Alarm silence	Available (except for beds connected via the QI-910R interface)	
Alarm recording	Available	

Trend

Trend parameters	Depends on the connected bedside monitor or transmitter
Trend display times	1, 8, 24, 72 h
Trend display formats	Trendgraph and tabular trend
Events related to trendgraph	ASYSTOLE, V FIB, V TACHY, VPC RUN, COUPLET, Off/Noise

Waveform Sensitivity

ECG display sensitivity	×1/4, ×1/2, ×3/4, ×1, ×1.5, ×2, ×4
Respiration curve sensitivity	×1/4, ×1/2, ×3/4, ×1, ×1.5, ×2, ×4
BP display scale (mmHg)	0-20, 0-50, 0-100, 0-200, 50-200, 50-250, 0-300 mmHg

Overview

Displays user-selectable vital signs, up to 12 ECG waveforms, trend data, alarm events, and status messages associated with the selected overview bed.
The overview bed can be any bed in the network that the central monitor is not continuously monitoring.

Remote Setting

Alarm setting of bedside monitors and multiple patient receivers
Individual setting of bedside monitors and multiple patient receivers
Channel setting of multiple patient receivers

Full Disclosure

Saves 72 hours of full disclosure waveform data for up to six waveforms and displays them on the Full Disclosure window.
(When the QP-973P Full Disclosure Filing Program Kit is installed.)

File Saving

Trend
Arrythmia recall file
Hemodynamic data list
ST recall

Full disclosure data (only when the QP-973P Full Disclosure Filing Program Kit is installed.)
ECG 12Lead analysis result filing (only when the QP-974P 12 Lead ECG Interpretation Filing Program Kit is installed.)
Caliper data

2-ch recorder, WS-971R (option)

Recording method	Thermal array recording
Number of channels	2
Recording paper	50 mm width (FQW50-3-100)
Paper speed	25 mm/s
Printed items	Patient information, date and time, waveform and measurement data, record type, paper speed
Record type	
Manual recording:	Delayed waveform recording, Freeze recording, Dual delayed waveform recording, Dual delayed waveform freeze recording, Arrhythmia recall recording, ST recall recording, Expanded full disclosure waveform recording
Automatic recording:	Periodic recording, Alarm recording
Call recording	
Remote delayed waveform recording	

Laser Printer (local purchase)

Paper size	A4/Letter
Record type	
Manual recording:	Multi-Wave printing, Multi-Wave Freeze printing, ECG 12 Lead printing, Trendgraph printing, Tabular Trend printing, Arrhythmia Recall recording, Hemodynamics List printing, ST Recall recording (ST recall files with printing mark), Full Disclosure Waveform printing, Expanded Full Disclosure Waveform printing, ECG 12 Lead Analysis Result printing, Report printing

Power Requirements

MU-971RA/RJ/RK Main Unit

Line voltage	AC 100 to 240 V ± 10%
Line frequency	50 or 60 Hz
Power consumption	AC 230VA or less

VL-971R/RK LCD Unit

Line voltage	AC 100 to 240 V ± 10%
Line frequency	50 or 60 Hz
Power consumption	AC 150VA or less

Environment

Operating temperature	10 to 35°C
Operating humidity	30% to 80% (no condensing)
Operating atmospheric pressure	70 to 106 kPa
Storage temperature	–20to +60°C
Storage humidity	20% to 90% (no condensing)
Storage atmospheric pressure	70 to 106 kPa

Electromagnetic Compatibility

MU-971RJ/RK main unit:	EMI	EN55022 C Class B
	Immunity	EN55024 1998
VL-971R/RK LCD Unit	IEC-60601-1-2 1993	

Safety

MU-971RA/RJ/RK main unit

Safety standard	IEC60950 3rd Ed.
Type of protection against electric shock	Class I
Degree of protection against electric shock	Type B applied parts
Degree of protection against harmful ingress of water	IPX0 (ordinary equipment)
Degree of safety of application in the presence of a flammable anaesthetic mixture with air, oxygen or nitrous oxide	Not suitable for use in the presence of a flammable anaesthetic mixture with air, oxygen or nitrous oxide
Mode of operation:	Continuous operation
Equipment types (classification)	Indoor stationary equipment

VL-971R/RK LCD Unit

Safety standard	IEC 60601-1 1995
Type of protection against electric shock	Class I
Degree of protection against electric shock	Type B applied parts
Degree of protection against harmful ingress of water	IPX1
Degree of safety of application in the presence of a flammable anaesthetic mixture with air, oxygen or nitrous oxide	Not suitable for use in the presence of a flammable anaesthetic mixture with air, oxygen or nitrous oxide
Mode of operation:	Continuous operation

Dimensions and Weight

Main unit	180 (W) × 352 (H) × 405 (D) mm, approx.16 kg
LCD unit (without protrusion)	457 (W) × 472 (H) × 247 (D) mm, approx.11 kg

Panel Descriptions

Central Monitor Main Unit MU-971RA/RJ/RK

WARNING

While the central monitor is on, do not insert any CD-ROM or floppy disk into it. Nihon Kohden does not warrant the normal operation of the central monitor in the case that an application or software installation starts automatically.

CAUTION

While the central monitor is on, do not touch unused sockets. Failure to follow this caution may damage the monitor by static electricity and may cause malfunction.

Front Panel

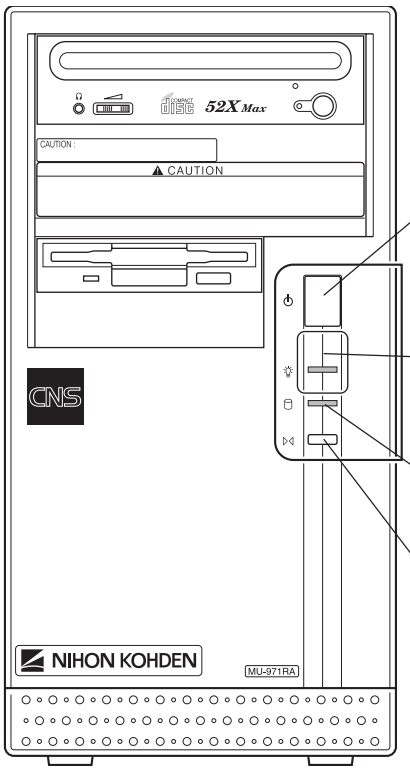

Power switch
Turns main unit on or off when the main power switch on the rear panel is on (|).

Power switch cover
For attaching, refer to CNS-9701 installation guide.

Hard disk lamp
Lights when the hard disk is being accessed.

Reset switch
Normally not used.

Rear Panel

NOTE

- **Do not remove the covers from the unused sockets on the rear panel of the central monitor main unit.**
- **Do not touch the sockets on the rear panel of the main unit or cables around the sockets. Otherwise, static electricity may cause malfunction of the monitor.**

<Volax5000> **<Volax5001>**

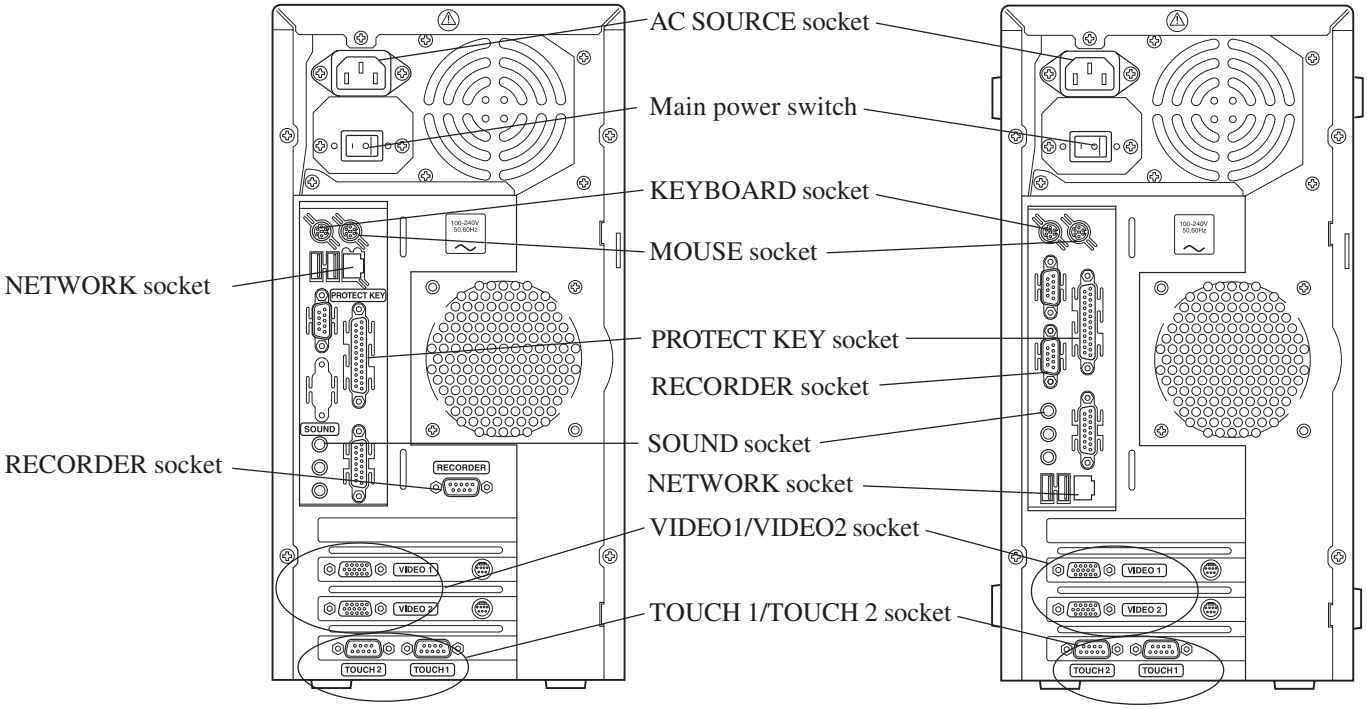

Name	Description
AC SOURCE socket	Connects to a UPS via the power cord provided with the central monitor main unit.
Main power switch	Turns on or off to supply power to the main unit. Under normal conditions keep this switch turned on (|).
KEYBOARD socket	Connects to the keyboard.
MOUSE socket	Connects to the mouse.
NETWORK socket	Connects to network system via a network cable.
SOUND socket	Connects to the SOUND socket on the VL-971R/RK LCD unit.
PROTECT KEY socket	Connects to the protection key via the connection cable provided with the central monitor main unit. This protection key can be connected to the protection keys for the QP-971P/972P/973P/974P program kits.
RECORDER socket	Connects to the WS-971R recorder unit.
VIDEO1/VIDEO2 socket	Connects to the VIDEO socket on the LCD unit via the RGB connection cable provided with the LCD unit.
TOUCH 1/TOUCH 2 socket	Connects the TOUCHSCREEN socket on the LCD unit via the touchscreen connection cable provided with the LCD unit.

LCD Unit VL-971R/RK

WARNING

Do not turn off the display to which the sound cable is connected. Otherwise alarm sound does not occur.

Front

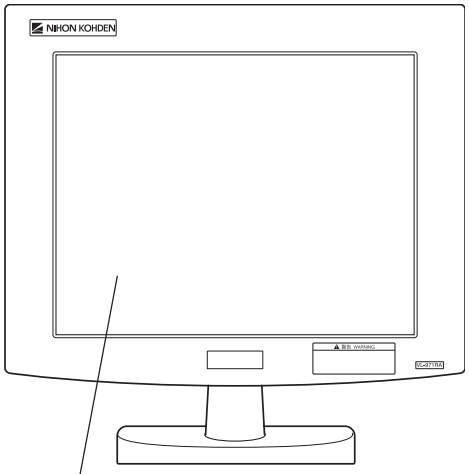

Touchscreen display

Rear

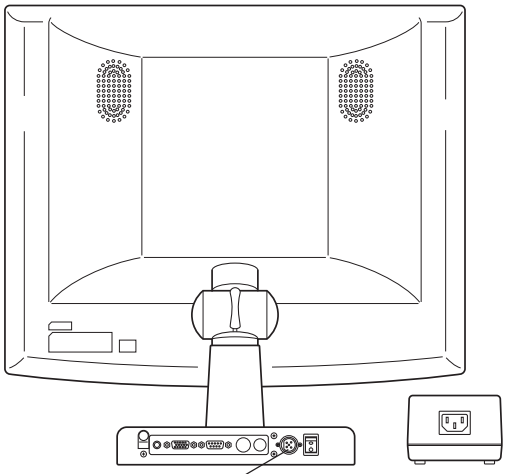

DC IN socket
Connects to the AC adapter cord

AC adapter (100 to 240 V)
Connects to a UPS via the power cord provided with the display unit.

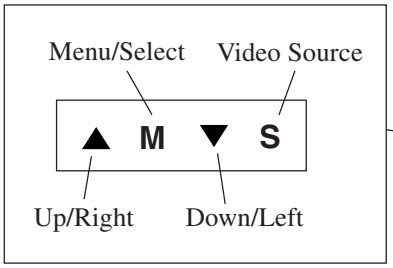

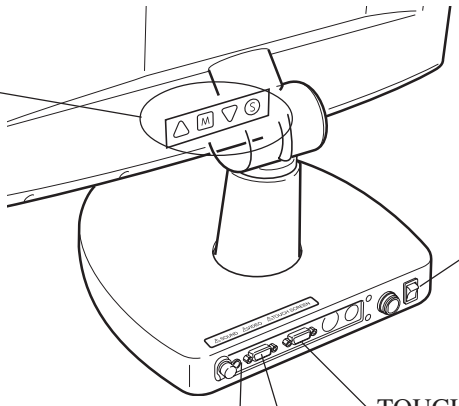

Power switch
Turns on (⊙) or off (◯) the LCD unit. Under normal conditions keep this switch turned on.

TOUCHSCREEN socket
Connects the TOUCH 1/TOUCH 2 socket on the central monitor main unit via the touchscreen connection cable provided with the LCD unit.

SOUND socket
Connects to the SOUND socket on the central monitor main unit via the sound cable provided with the central monitor.

VIDEO socket
Connects to the VIDEO1/VIDEO2 socket on the central monitor main unit via the RGB connection cable provided with the LCD unit.

Recorder Unit WS-971R

POWER lamp
Lights when the power is on.

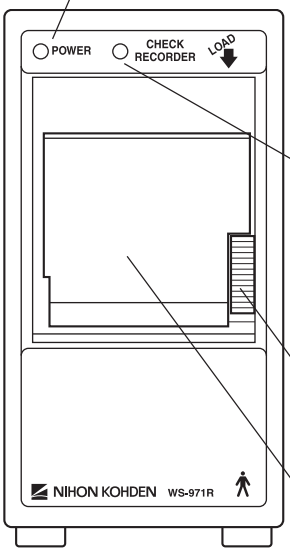

CHECK RECORDER lamp
Lights when communication between the recorder unit and central monitor is disconnected or when there is abnormality in the recorder unit.

Paper magazine release lever
Press to open the magazine.

Paper magazine
Contains the recording paper.

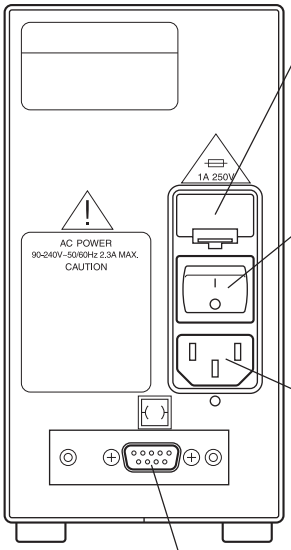

Fuse holder
Two fuses (1A) are contained. Fuse must be replaced by qualified service personnel.

Power switch
Turns the power ON (|) or OFF (○).
Usually, keep the power ON.

Power socket
Connects to a UPS with a power cord provided with the central monitor main unit and supplies power (100 to 240 V) to the recorder unit.

PC socket
Connects to the RECORDER socket on the rear panel of the central monitor main unit with the recorder cable provided with the central monitor main unit.

Composition

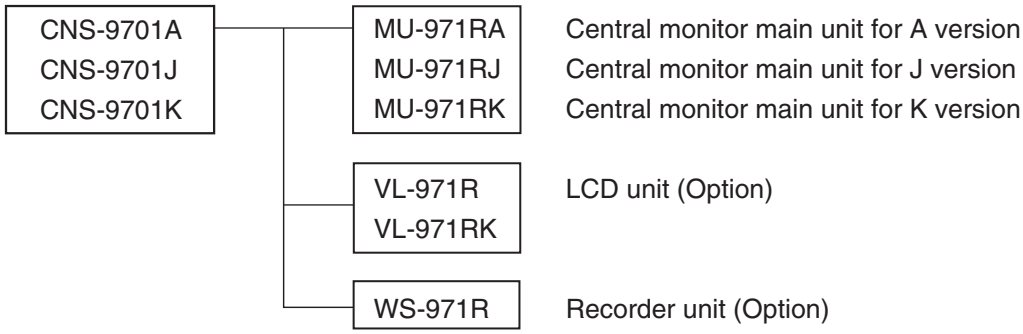

Options

QP-971P	12 Patient Examination Program Kit
QP-972P	16 Patient Examination Program Kit
QP-973P	Full Disclosure Filing Program Kit
QP-974P	12 Lead ECG Interpretation Filing Program Kit

Connection Diagram

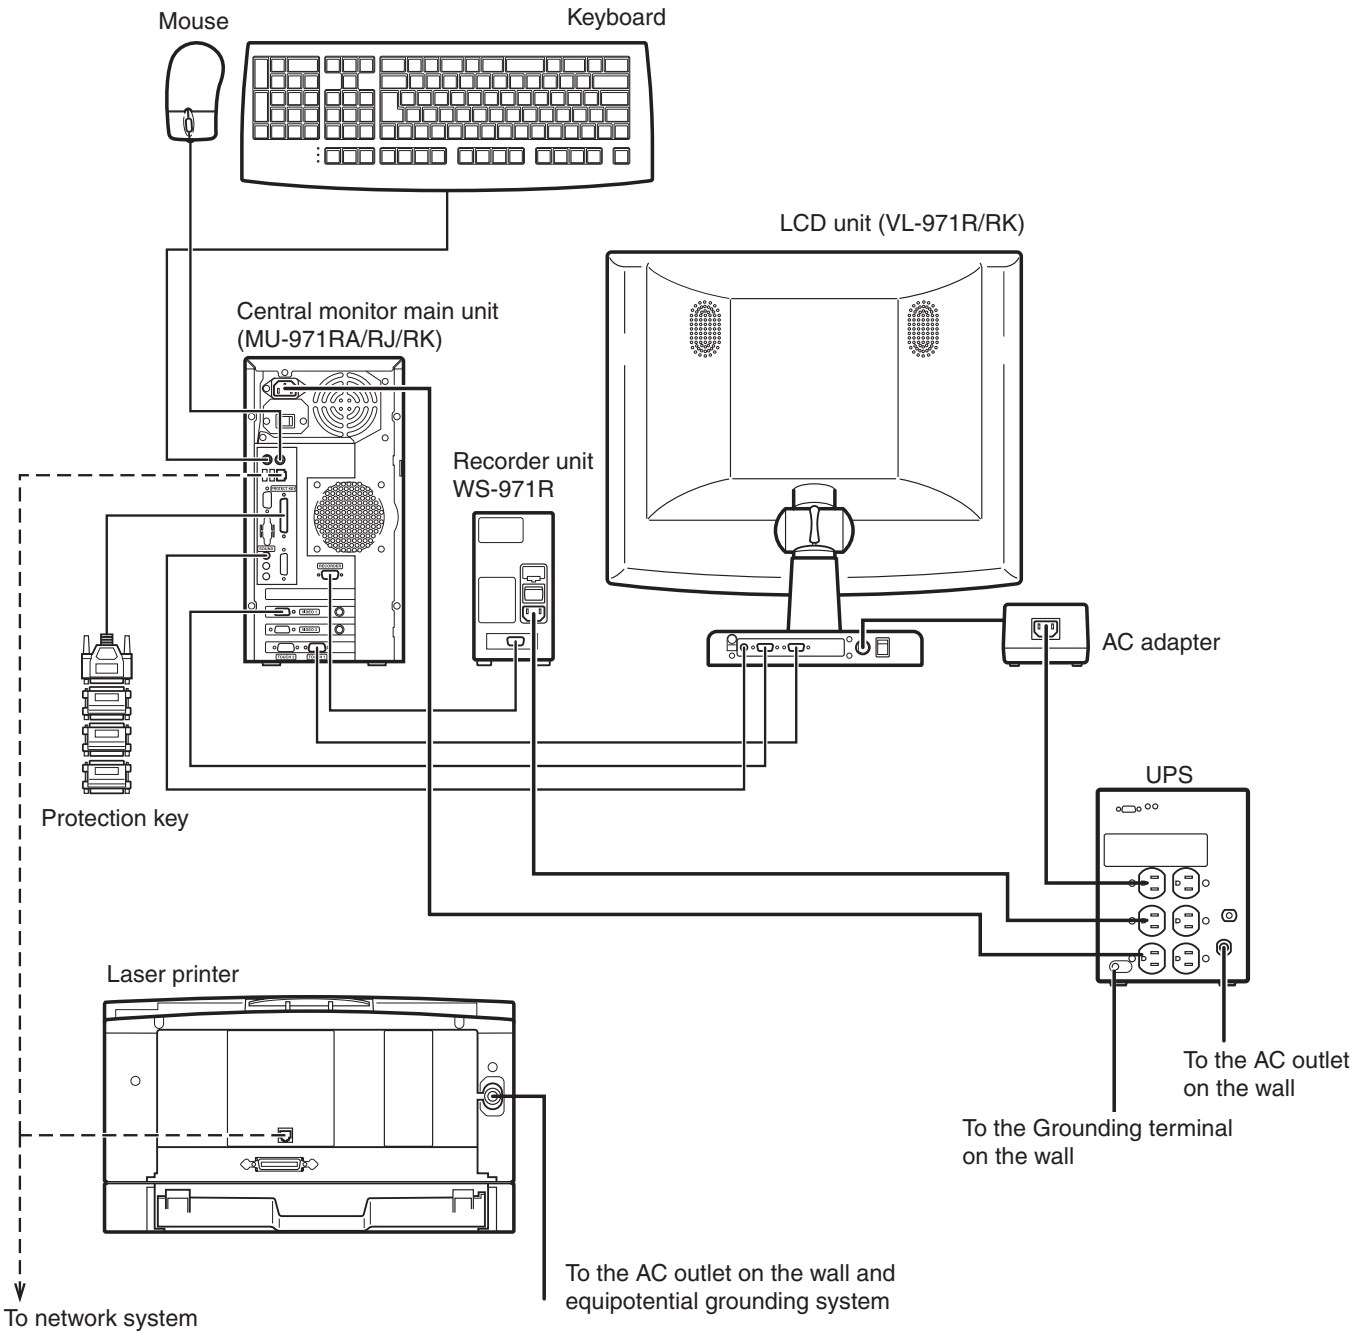

When using two displays

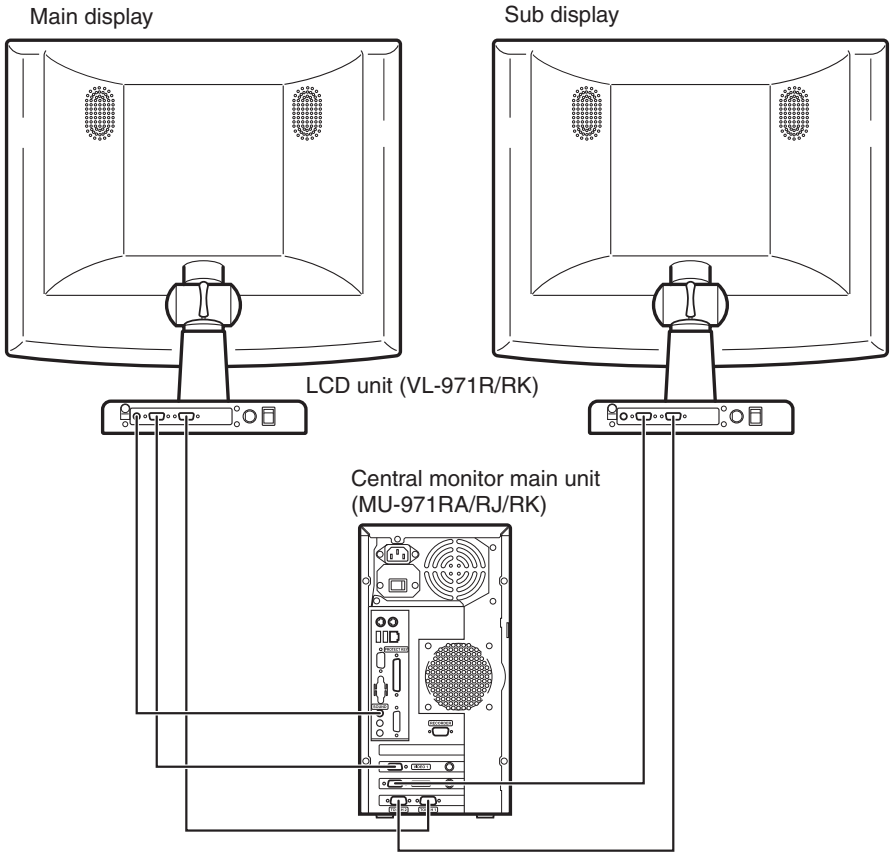

Section 2 Troubleshooting

General 2.1
System 2.3
Network 2.4
Measurement Value 2.5
Alarm 2.5
Admitting/Discharging 2.6
All Beds Screen/Individual Bed Screen 2.7
Trend Window 2.8
Tabular Trend Window 2.8
Hemodynamics List Window 2.8
Arrhythmia Recall Window 2.9
ST Recall Window 2.9
Full Disclosure Window 2.10
ECG 12 Lead Analysis Window 2.10
Report Window 2.11
Recording 2.11
Overview Bed Screen 2.12
Parameter Setup 2.12
Power Problem 2.13
Display Problem 2.14
Touch Screen Problem 2.16
Sound Problem 2.16
Keyboard Problem 2.17
Mouse Problem 2.17
Hard Disk Problem 2.17
CD-ROM Drive or Floppy Disk Drive Problem 2.18
2-channel Recorder Unit Problem 2.18
Error Messages 2.19
- Messages From Bedside Monitors/Multiple Patient Receiver 2.19
  - Messages about Measurement Conditions of Each Parameter 2.19
  - Other 2.24
- Messages From Central Monitor 2.25
  - WS-971R Recorder Unit 2.25
  - Laser Printer 2.25

Other 2.25
Hard Disk Replacement Flow 2.26
How to Recover the BIOS Initial Settings 2.27
BIOS Default Setting (Vorax5000) 2.28
BIOS Default Setting (Vorax5001) 2.30

General

Use the troubleshooting tables to locate, identify, and solve a problem in the instrument. The problems are divided into general problem areas. Each category has its own troubleshooting table for fast and easy troubleshooting.

- System
- Network
- Measurement Value
- Alarm
- Admitting/Discharging
- All Beds Screen/Individual Bed Screen
- Trend Window
- Tabular Trend Window
- Hemodynamics List Window
- Arrhythmia Recall Window
- ST Recall Window
- Full Disclosure Window
- ECG 12 Lead Analysis Window
- Report Window
- Recording
- Overview Bed Screen
- Parameter Setup
- Power Problem
- Display Problem
- Touch Screen Problem
- Sound Problem
- Keyboard Problem
- Mouse Problem
- Hard Disk Problem
- CD-ROM Drive or Floppy Disk Drive Problem
- 2-channel Recorder Unit Problem

If these sections do not solve the problem, contact your Nihon Kohden representative.

NOTE

Before contacting your Nihon Kohden representative for technical support, please provide additional detailed information on the problem. This will allow your Nihon Kohden representative to provide you with the best support.

How to use the troubleshooting table

1. Determine which troubleshooting table to use.

2. In the “Problem” column, find the trouble item that matches the problem.

3. Do the action recommended in the “Action” column.

4. If the problem is not solved, do the action for the next possible cause or criteria.

5. If none of the actions solve the problem, contact your Nihon Kohden representative.

System

Trouble	Possible Cause/Criteria	Action
The touch screen keys do not function.	The pressed position and activated position do not match.	Reboot the display with the following procedure. 1. Confirm the cable connection for the touch screen. 2. Turn off the LCD display and then turn it on again. 3. Perform touch screen initialization and calibration at the Touchscreen Setting window of the System Setup. If the trouble remains after actions 1 to 3, exit the central monitor program and restart Windows 2000.
The mouse disappears off the screen.	The central monitor is operated in dual display mode.	To stop dual display mode, do the following: 1. On the Monitor Setting window of the System Setup, set "Number of Displays" to Single Display. 2. On the Display Properties window of Windows 2000, set "Display2" to OFF, then reboot the system.
The "System Setup" key cannot be touched.	The central monitor is operated in dual display mode and the System Setup screen is open at the other display.	
Display position is not correct.	The screen is out of synchronization.	VL-971R/RK LCD unit: Set the correct screen frequency using the smart synchronization function. Locally purchased LCD unit: Select the correct screen frequency referring to the LCD unit operation manual.
No display on the second display	Settings on the Display Properties window of Windows 2000 are not set properly.	On the Display Properties window of Windows 2000, set "Display2" to ON, then reboot the system. (When the product is shipped, this setting is set to OFF.)
An application error occurs when you start the central monitor system program and the system does not start.		Confirm that the Display Properties window of Windows 2000 is set as below. When the central monitor is operated in the dual display mode, confirm both display 1 and 2. Screen Area: 1280 × 1024 Colors: True color On the Windows setting window, set display 1 to the left and 2 to the right.
Cannot display data saved in the NFS-9000 network file server.	---	At present, the CNS-9701 central monitor cannot display data saved in the NFS-9000 network file server.

Trouble	Possible Cause/Criteria	Action
Data is deleted when the central monitor power is turned off.	Faulty hard disk	Contact your Nihon Kohden distributor or representative. The central monitor may lose its function as a monitor.
The system crashes when trying to review the past data.		
The system crashes periodically such as once a day.		
Incorrect date and time	Clock error	Contact your Nihon Kohden distributor or representative.
	If the clock becomes incorrect after adjusting the clock and turning the central monitor power on again, the back up battery is weak.	
• Slow operation • It takes time to read out the saved data. • Malfunction	Windows is unstable.	Shut down the central monitor system program and restart it. For a stable operation, restart the central monitor system program once every three months.

Network

Trouble	Possible Cause/Criteria	Action
A desired bed is not displayed in the selected group.	The bedside monitor or multiple patient receiver for that bed is turned off.	Turn on the bedside monitor or multiple patient receiver.
	The desired bed belongs to another group.	On the Monitor Setting window, check other groups to find the desired bed. Check group names of each bedside monitor and multiple patient receiver.
Cannot find 8000 series beds in the network	---	8000 series beds connected to the network via the CNS-9301/9302 central monitor belong to the same group as the CNS-9301/9302 central monitor.
The lamp near the NETWORK socket on the main unit does not light and the main unit cannot communicate with any instrument connected to the network.	The network cable is loose at the socket.	Check that the network cable and its connectors at both ends have no damage and check the continuity. After these checks, firmly connect the cable between the main unit and hub.
	The network circuit on the motherboard has a failure.	Replace the motherboard with a new one.
	The hub connected to the main unit through the network cable has a failure.	Replace the hub with a new one.

Measurement Value

Trouble	Possible Cause/Criteria	Action
Heart rate is not counted correctly.	Waveform too large or too small	Adjust the QRS detection sensitivity.
	QRS detection threshold is changed.	
	QRS and pacemaker spikes are not distinguished.	Turn pacing detection ON.
	QRS detection is set to “Manual”.	Set QRS detection to “Auto”, or confirm that the QRS detection lead and threshold in manual detection are set properly.
Arrhythmia is not measured correctly.	ECG learning is not correct.	Relearn patient’s ECG.
Heart rate and arrhythmia are not measured correctly.	ECG lead that is inappropriate for analysis is selected.	Change the ECG lead used for analysis.
Noise on the ECG waveform	Hum interference on the ECG waveform.	Set the hum filter to ON.
The ST value is inaccurate.	The ST analysis point is not set properly.	Confirm that the ST analysis point setting is properly set for ST analysis.
Respiration is not measured correctly.	Waveform too large or too small	Set the proper sensitivity.
	Respiration sensitivity is changed.	
	Respiration measurement is set to OFF.	Turn the respiration measurement ON.

Alarm

Trouble	Possible Cause/Criteria	Action
No alarm.	Each alarm setting of the Personal Setup is set to OFF.	Turn the alarms ON for the bed.
	Arrhythmia analysis is turned OFF at the bedside monitor and/or central monitor.	Turn arrhythmia analysis ON on both the bedside monitor and central monitor.
	All alarms are set to OFF at the bedside monitor.	Turn all alarms ON at the bedside monitor. This operation cannot be done at the central monitor.
All alarms for a bed cannot be turned ON/OFF together.	---	This operation is not available at the central monitor.

Admitting/Discharging

Trouble	Possible Cause/Criteria	Action
Cannot transfer a patient's data.	You are trying to do this operation on a central monitor where the patient's data is not saved.	Do this on the central monitor where the patient's data is saved.
Cannot change the receiving channel.		
Cannot admit/discharge a patient.	You are trying to do this operation on a central monitor where the patient's data is not saved.	Do this on the central monitor where the patient's data is saved.
	The bedside monitor is turned off.	Turn on the bedside monitor.
Cannot select a bedside monitor as a transfer destination bedside monitor.	The bedside monitor is turned off.	Turn on the bedside monitor.
The patient's data before patient transfer is lost.	The patient was transferred between bedside monitors in different CNS groups more than once.	To save the patient's data in the first central monitor, do not transfer the patient to a bedside monitor in a third CNS group after the patient is transferred to a bedside monitor in a second CNS group.
The patient's data before patient transfer cannot be reviewed.	The central monitor where the patient's data is saved is turned off.	Turn on the central monitor where the patient's data before the patient transfer is saved.
The message "Transferring" is displayed on the screen but it does not change to "Completed".	During patient transfer, the central monitor was turned off. Or, there was trouble on the network and the transfer failed.	Admit the patient at the destination bedside monitor. The lost data cannot be restored.
All patient's data is lost after patient transfer.		
ST recall data is lost after patient transfer.	You transferred an 8000 series bed that was a monitored bed of a CNS-9301/9302 central monitor.	You cannot transfer ST recall data of an 8000 series bed that was a monitored bed of a CNS-9301/9302 central monitor.

All Beds Screen/Individual Bed Screen

Trouble	Possible Cause/Criteria	Action
Numeric data and messages disappear for a moment.	The display is refreshed. This is normal.	---
Waveform is not displayed.	The bed is discharged.	Admit the patient.
	The bed is set to temporary discharge.	Resume monitoring.
	The bedside monitor or the multiple patient receiver is turned off.	Turn on the bedside monitor or the multiple patient receiver.
	The currently measured lead/label is different from the lead/label to be displayed on the screen.	Confirm the setting so that the currently measured lead/label matches the lead/label to be displayed on the screen.
	The waveform is not selected as the displayed waveform.	Set the waveform to the displayed waveform.
	The bed is not registered as a monitored bed.	Register the bed to the monitored bed.
	Network is disconnected.	Confirm the network connection.
	The bedside monitor is an 8000 series bed connected to the network via the CNS-9301/9302 central monitor.	Several types of waveforms cannot be displayed on 8000 series bedside monitors.
Numeric data is not displayed.	The parameter of the numeric data is not selected as the displayed parameter.	Set the parameter of the numeric data to the displayed parameter.
	The label of the currently measured numeric data is different from the label to be displayed.	Confirm the setting so that the label of the currently measured numeric data matches the label to be displayed.
	A vital alarm occurred in a parameter that is not set to a displayed parameter and its numeric data took the place of a numeric data that is set to the displayed parameter.	The numeric data of a parameter whose vital alarm is currently occurring has a higher priority to be displayed.
The desired waveform or numeric data cannot be selected.	The waveform or numeric data is not measured.	Measure the waveform or numeric data.
		Confirm the setting so that the currently measured lead/label matches the lead/label to be displayed on the screen.
		Register the desired parameter on the Parameters window of the System Setup. A parameter registered at the Parameters window of the System Setup is displayed on setting keys even when it is not currently measured.
Some waveforms are not displayed.	Some of the patient waveforms cannot be displayed on this central monitor while another central monitor that is connected to a multiple patient receiver or a signal exchanger displays the individual bed screen of the patient.	Display the All Beds screen at the central monitor where the patient's data is saved.
The desired parameter cannot be displayed.	The parameter is a parameter that cannot be displayed.	Refer to Section 15 "Parameter Priority" for the list of parameters that can be displayed on the central monitor.
Cannot find a key to freeze a waveform or relearn ECG.	Those functions are not assigned to function keys.	Assign these functions to function keys.

Trend Window

Trouble	Possible Cause/Criteria	Action
Trend data is not displayed.	The central monitor where the bed's data is saved is turned off.	Turn on the central monitor where the bed's data is saved.
Trend data is not saved.	The central monitor where the bed's data is saved was turned off during measurement.	Trend data is not created when the central monitor where the bed's data is saved is turned off.

Tabular Trend Window

Trouble	Possible Cause/Criteria	Action
Tabular trend data is not displayed.	The central monitor where the bed's data is saved is turned off.	Turn on the central monitor where the bed's data is saved.
Cannot select a parameter you want to add to the tabular trend	The parameter is not registered at the Parameters window of the System Setup.	Register the parameter at the Parameters window of the System Setup.
NIBP numeric data is not displayed.	When an NIBP measurement is delayed or remeasured and its measurement timing does not match the selected tabular trend interval, that NIBP data will not appear on the tabular trend.	Set the tabular trend display interval to 1 min. The NIBP tabular trend and all NIBP measurements are displayed.
Tabular trend data is not saved.	The central monitor where the bed's data is saved was turned off during measurement.	Tabular trend data is not created when the central monitor where the bed's data is saved is turned off.

Hemodynamics List Window

Trouble	Possible Cause/Criteria	Action
Hemodynamics data is not displayed.	The central monitor where the bed's data is saved is turned off.	Turn on the central monitor where the bed's data is saved.
Hemodynamics data is not saved.	The central monitor where the bed's data is saved was turned off during measurement.	Hemodynamics data is not created when the central monitor where the bed's data is saved is turned off.
	The bedside monitor cannot output hemodynamics data to the network.	Hemodynamics data that can be reviewed at the central monitor is data created at the BSM-4100 series bedside monitor version 02-09 or later.

Arrhythmia Recall Window

Trouble	Possible Cause/Criteria	Action
Arrhythmia recall files are not created.	The arrhythmia analysis is set to OFF.	Turn the arrhythmia analysis to ON.
Arrhythmia recall files for a particular arrhythmia are not created	Recall file creation for the arrhythmia is set to OFF.	Turn the setting to ON.
Arrhythmia recall files for unnecessary arrhythmias are created.	Recall file creation for the arrhythmia is set to ON.	Turn the setting to OFF.
Arrhythmia recall files are deleted.	The number of arrhythmia recall files for one bed exceeded the limit and older files are deleted.	Deleted files cannot be recovered.
	You touch “Delete” when several files have a deletion mark.	
Arrhythmia recall files are not displayed.	The bedside monitor is turned off.	Turn the bedside monitor or multiple patient receiver on.
	The central monitor where the bed’s data is saved is turned off.	Turn on the central monitor where the bed’s data is saved.
	The arrhythmia types to be displayed on the screen are not selected.	Select the arrhythmias to be displayed on the screen.
Arrhythmia recall files are not saved.	The central monitor where the bed’s data is saved was turned off during measurement.	Arrhythmia recall files are not created when the central monitor where the bed’s data is saved is turned off.
When the multi waveform display is selected, the desired waveforms cannot be displayed.	Stored waveforms and displayed waveforms are not selected for full disclosure waveform.	Waveforms displayed for the multi waveform display are synchronized with the displayed waveform settings on the Full Disclosure window. Set at “Stored Waves” and “Displayed Waves” on the Full Disclosure window.
Multi waveform cannot be displayed.	The QP-973P Full Disclosure Filing Program Kit is not installed.	Install the QP-973P Full Disclosure Filing Program Kit.

ST Recall Window

Trouble	Possible Cause/Criteria	Action
ST recall files for 72 hours cannot be saved.	The interval of ST recall file creation is set to 30 seconds.	With the creation interval of 30 seconds, the total number of files exceeds the limit. To save recall file for 72 hours, set the creation interval to 1 min or more.
ST recall files are not saved.	The central monitor where the bed’s data is saved is turned off.	Turn on the central monitor where the bed’s data is saved.
	The bedside monitor cannot output ST recall files to a network.	The central monitor cannot save or display ST recall files of the following bedside monitors: • BSM-4100 series bedside monitor whose version is not 02-09 or later • 8000 series bed that is a monitored bed of a CNS-9301/9302 central monitor.

Full Disclosure Window

Trouble	Possible Cause/Criteria	Action
Full disclosure waveform is not displayed.	The central monitor where the bed's data is saved is turned off.	Turn on the central monitor where the bed's data is saved.
	The QP-973P Full Disclosure Filing Program Kit is not installed.	Install the QP-973P Full Disclosure Filing Program Kit.
	The QP-973P Full Disclosure Filing Program Kit is not installed in the central monitor where the bed's data is saved.	Choose a central monitor with the QP-973P Full Disclosure Filing Program Kit installed for the central monitor where the bed's data is saved.
The desired full disclosure waveform is not displayed.	The full disclosure waveform is not saved.	Choose the waveform for the stored waveform on the Full Disclosure window.
The desired waveform cannot be selected for a stored waveform.	The parameter is not measured.	Measure the parameter.
	This central monitor is not the central monitor where the bed's data is saved.	This setting is only available at the central monitor where the bed's data is saved or the BSS-9800 bedside station (central mode).
The waveforms that are selected for the stored waveform are not saved.	The central monitor where the bed's data is saved was turned off during measurement.	Full disclosure waveform is not saved when the central monitor where the bed's data is saved is turned off.
	The currently measured lead/label is different from the lead/label to be saved.	Make the currently measured lead/label match the lead/label to be saved.
On the Full Disclosure window, the arrhythmia waveform is not indicated with the preset color.	Arrhythmia analysis is set to OFF at the bedside monitor and/or the central monitor.	Turn arrhythmia analysis to ON at the bedside monitor and central monitor. You cannot set color to an arrhythmia that does not have color.
	The arrhythmia alarm is set to OFF at the bedside monitor and/or the central monitor.	Turn the arrhythmia alarm to ON at the bedside monitor and central monitor. You cannot set color to an arrhythmia that does not have color.
	Noise interference Poor electrode attachment condition	You cannot set color to an arrhythmia that does not have color.

ECG 12 Lead Analysis Window

Trouble	Possible Cause/Criteria	Action
ECG 12 Lead analysis files are not displayed.	The QP-974P 12 Lead ECG Interpretation Filing Program Kit is not installed.	Install the QP-974P 12 Lead ECG Interpretation Filing Program Kit.
	The bedside monitor cannot output ECG 12 lead analysis files to a network.	The central monitor can display ECG 12 lead analysis files of the BSM-4100 series bedside monitor only when the bedside monitor version is 03-02 or later.

Report Window

Trouble	Possible Cause/Criteria	Action
Report printing starts automatically.	The report printing mode is set to “Auto”.	Set the mode to “Manual”.

Recording

Trouble	Possible Cause/Criteria	Action
In the following recordings, waveforms that you do not want to record are recorded. - Manual recording - Periodic recording - Alarm recording - Call recording	Waveforms displayed on the All Beds screen are recorded.	---
In the following recording, waveforms that you do not want to record are recorded. - Dual waveform recording	Recorded waveform is not selected on the Recording window of the Setup.	Select the desired waveform on the Recording window of the Setup.
In the following recording, waveforms that you do not want to record are recorded. - Remote delayed waveform recording	Recorded waveform is selected at the bedside monitor.	---
Alarm recording is not performed for a particular arrhythmia.	Recall file creation for the arrhythmia is set to OFF.	Turn the setting to ON.
Vital sign alarm recording is not performed.	Vital sign alarm recording is set to OFF.	Set vital sign alarm recording to ON.
Arrhythmia alarm recording is not performed.	Arrhythmia alarm recording is set to OFF.	Set arrhythmia alarm recording to ON.
	Arrhythmia analysis is set to OFF at the bedside monitor.	Turn arrhythmia analysis to ON at the bedside monitor.
ST alarm recording is not performed.	ST alarm recording is set to OFF.	Set ST alarm recording to ON.
Periodic recording is not performed.	Periodic recording is set to OFF on the Recording window of the Setup.	Set periodic recording to ON.
Call recording is not performed.	Call recording is set to OFF on the Recording window of the Setup.	Set call recording to ON.
Trend data are not printed for the report printing.	Report settings are not correct.	Set the correct settings on the Report window.
Dual waveform recording is not performed. (Only one waveform is recorded/printed.)	On the Recording window of the Setup, “Second Wave” at “Recording Pattern” is set to NONE.	Set a desired waveform for “Second Wave” at “Recording Pattern”.
Waveform is not printed on the screen copy.	Waveform cannot be printed on the screen copy.	---

Overview Bed Screen

Trouble	Possible Cause/Criteria	Action
Some waveforms are not displayed.	When the individual bed screen of a patient is displayed on a central monitor that is connected to a multiple patient receiver or a signal exchanger, some of the patient waveforms cannot be displayed on the Overview Bed of another central monitor.	Display the All Beds screen at the central monitor that saves the data of the bedside monitor you want to display.
The desired bed cannot be selected for the Overview Bed screen.	The bed is an 8000 series bed.	To display data of an 8000 series bed on this central monitor, a central monitor on the network must be monitoring the bed.
The alarm for the overview bed does not occur.	No bedside monitor is selected at the Overview Bed screen.	Select a desired bed as an overview bed.
Cannot silence an overview bed alarm.	An overview bed alarm cannot be silenced at the central monitor.	To stop overview bed alarm, stop monitoring any overview bed by touching “Stop monitoring” on the Overview Bed Menu screen.
An overview bed alarm of an unintended bed occurs.		

Parameter Setup

Trouble	Possible Cause/Criteria	Action
Available settings differ among bedside monitors.	Available settings depend on the bedside monitor model and connection method.	---

To replace the board or unit with a new one, refer to Section 4 “ Disassembly and Assembly”.

Power Problem

Problem	Possible Cause	Action
- When the main unit is turned on, the power lamp on the front panel does not light. - When the display unit is turned on, the LCD does not light. - The main unit or display unit frequently turns itself off.	AC power is not obtained from the power cord.	Check that the AC power is obtained from the AC outlet on the facility wall.
	The power cord is loose between the AC outlet and AC inlet of the main unit or display unit through the AC adapter.	Disconnect the power cord between the AC outlet and AC inlet of the main unit or AC adapter, and connect the power cord between them again.
	The power supply unit in the main unit or AC adapter for the display unit has a failure.	Replace the power supply unit or AC adapter with a new one.
In power failure, the UPS does not cover the power requirement of the central monitor.	The battery in the UPS is completely discharged.	Replace the battery with a new one.
	UPS has a failure.	Replace the UPS with a new one.

Display Problem

CAUTION

To replace the hard disk with a new one, refer to "Hard Disk Flow" in this section and "Replacing the Hard Disk" in Section 4 "Disassembly and Assembly".

Problem	Possible Cause	Action
The "NO SIGNAL" message appears on the black screen of the display unit.	The RGB cable has poor contact between the display unit and main unit.	Disconnect the RGB cable and firmly connect the RGB cable between them.
	The RGB signals are not output from the graphic board in the main unit.	Replace the graphic board with a new one.
	The main unit is not turned on.	Check the problem items shown in the above "Power problem" table.
- The screen is out of synchronization. - The screen is flickering. - The screen display position is not correct.	The horizontal or vertical synchronization setting is not adjusted properly.	Perform the synchronization adjustment at the display unit.
A "No boot device" message appears and Windows 2000 does not start.	The hard disk is damaged.	Replace the hard disk with a new one.
	The hard disk is not recognized due to incorrect BIOS setting.	Set the BIOS setting correctly.
A "HDD Problem Call Nihon Kohden" message appears and the hard disk lamp is lit.	The hard disk is damaged.	Replace the hard disk with a new one. (To use the central monitor temporarily, turn the main unit off and on. But note that this problem will appear again some time.)
The screen is only one color such as - The screen color is only blue. - The screen color is only red. - The screen color is only yellow.	The RGB cable has an internal break.	Check the continuity with a multimeter. Replace the cable with a new one if the cable has a break.
	The graphic board in the main unit has a failure.	Replace the board with a new one.
	The display unit has a failure.	Replace the unit with a new one.
- The screen is not clearly displayed. - The screen display position varies. - The screen is distorted. - The screen dims.	Adjustment*[1] of the display unit is required.	Adjust the display unit according to "Adjustment" section.
	A failure of the display unit*[2] or graphic board of the main unit.	Replace the defective board*[3] with a new one.

Problem	Possible Cause	Action
- The display color balance has something wrong. - The screen background color is not black.	A failure of the display unit*2 or graphic board of the main unit.	Replace the defective board*3 with a new one.
	Internal break in the RGB cable	Check the continuity with a multimeter. Replace the cable with a new one if the cable has a break.
	Adjustment*1 of the display unit is required.	Adjust the display unit according to "Adjustment" section.
No screen is displayed but the backlight lamp is not lit.	Failure of the AC adapter in the display unit.	Check that the AC adapter outputs +12 V. If this voltage is not output, replace the AC adapter with a new one.
	Failure of the backlight lamp or inverter of the LCD assembly.	Replace the LCD assembly with a new one.
No screen is displayed but the backlight lamp is lit.	If NDS logo appears at the center of the screen when you turn on the display unit only, the display unit works.	Check that the RGB signals are output from the main unit. Adjust the display unit synchronization according to the "Adjustment" section.
	If NDS logo does not appear at the center of the screen when you turn on the display unit only, the display unit does not work.	Replace the LCD control board or LCD assembly with a new one.

*1 The VL-971R display unit is adjusted at the factory so that the display unit accepts the RGB signals from most of the RADEON graphic boards used in the main unit. But some of the boards require adjustment of the display unit.
*2 Most of these problems can be caused by a failure of the LCD control board in the display unit because the RGB outputs from the graphic board are controlled by an IC on the graphic board.
*3 To judge which board has a failure, connect another PC to the display unit or another RGB display unit to the main unit.

Touch Screen Problem

Problem	Possible Cause	Action
The touch screen does not work.	The RS232C straight cable has poor contact between the display unit and main unit.	Check the continuity of the cable with a multimeter and check the connection.
	The touch screen control board has a failure.	Replace the board with a new one.
	The touch screen is damaged.	Replace the touch screen with a new one.
	The film cable of the touch screen has a break.	
- Effective area varies on the touch screen. - The touch screen sometimes works.	The touch screen control board has an error due to noise.	Turn off the display unit and turn it on to initialize the display unit. If there is still the same problem or it occurs again, replace the board with a new one.
The pressed position and activated position do not match.	The display unit is moved to upper or lower location.	Calibrate the touch screen at the Touchscreen Setting window of the System Setup.
	The position data is changed by noise.	

Sound Problem

Problem	Possible Cause	Action
The main unit intermittently generates a beep sound.	A key on the keyboard is pressed and held.	Release the key.
No alarm and QRS sounds.	Poor contact of the speaker cable.	Check the continuity of the speaker cable and connector connection.
	Failure of the speakers in the display unit.	Replace the speakers with new ones.
	Failure of the motherboard in the main unit.	Replace the motherboard with a new one.
Abnormal low noise from the main unit.	Dust or lint on the cooling fan for the CPU or in the power supply unit.	Clean the fans with an air compressor.

Keyboard Problem

Problem	Possible Cause	Action
No keyboard keys work.	The keyboard cable is loose at the socket on the main board.	Disconnect the cable from the socket on the main board and connect the cable to the socket tightly.
	The keyboard cable is damaged.	Replace the keyboard with a new one.
Some keyboard keys do not work.	Failure of the key switches.	Replace the keyboard with a new one.

Mouse Problem

Problem	Possible Cause	Action
When you move the mouse, the cursor on the screen does not move.	The mouse cable is loose at the socket on the main unit.	Disconnect the cable from the socket on the main board and connect the cable to the socket tightly.
	Mouse failure.	Replace the mouse with a new one.

Hard Disk Problem

CAUTION

To replace the hard disk with a new one, refer to "Hard Disk Flow" in this section and "Replacing the Hard Disk" in Section 4 "Disassembly and Assembly".

Problem	Possible Cause	Action
A "No boot device" message appears and Windows 2000 does not start.	The hard disk is damaged.	Replace the hard disk with a new one.
	The BIOS setting is changed by noise so the hard disk is not recognized.	Set the correct BIOS setting again.
A "HDD Problem Call Nihon Kohden" message appears and the hard disk lamp is lit.	The hard disk is damaged.	Replace the hard disk with a new one. (To use the central monitor temporarily, turn the main unit off and on. But note that this problem will appear again some time.)
Following to the shut down procedure in the operator's manual, you shut down the central monitor but the screen does return to Windows 2000.	The hard disk is damaged.	Replace the hard disk with a new one.
Metallic sound from the hard disk.	The bearing for the spindle motor in the hard disk is worn out.	Replace the hard disk with a new one.

CD-ROM Drive or Floppy Disk Drive Problem

Problem	Possible Cause	Action
The access lamp lights but the drive cannot read the data on a disk.	The drive is dusty.	Clean the drive with a cleaning disk or air compressor.
The access lamp does not light during access and the drive cannot read the data on a disk.	The drive has a failure.	Replace the drive with a new one. After replacement, check that the new drive is recognized when the main unit is turned on.
	Poor connection between the drive and motherboard.	Check the connection between the drive and motherboard.

2-channel Recorder Unit Problem

Problem	Possible Cause	Action
The recording paper is loaded but the “RECORDER OUT OF PAPER” message appears on the screen.	The paper detection sensor is dirty.	Clean the paper detection sensor with a cotton swab moistened with alcohol.
The printing intensity is not even.	The platen roller is worn out.	Replace the roller with a new one.
The paper magazine is completely closed but the “RECORDER DOOR OPEN” message appears on the screen.	The magazine open detection switch has a failure.	Replace the switch with a new one.
Missing dot on recordings from the recorder unit.	The thermal array head has a failure.	Replace the head with a new one.

Error Messages

Error messages are categorized into two types, messages sent from bedside monitors/multiple patient receiver and messages generated at the central monitor.

Messages From Bedside Monitors/Multiple Patient Receiver

Messages about Measurement Conditions of Each Parameter

The central monitor receives error messages from bedside monitors and multiple patient receiver and displays them on the screen. Here is the message list. For causes and countermeasures for each message, refer to the bedside monitor/ multiple patient receiver operator's manual.

Some messages displayed at the bedside monitor/multiple patient receiver are not displayed on the central monitor.

Parameter	Message
ECG	CHECK LEADS
	CHG ELECTRODE
	NOISE
	SMALL QRS
	RHYTHM CHG
	LEARNING
	LOW mV
	HIGH mV
	AUTO LEAD CHG
	CANNOT ANALYZE
	PACING

Parameter	Message
Arrhythmia	ASYSTOLE
	V.FIB
	Vf/VT
	EXT.TACHY
	EXT.BRADY
	V.TACHY
	VPC RUN
	COUPLET
	EARLY VPC
	MULTIFORM
	BIGEMINY
	FREQ.VPC
	TACHYCARDIA
	BRADYCARDIA
	PROLONGED RR
	FREQ.SVPC
	NON-FUNCTION
	NON-CAPTURE
	PACE FAILURE
	IRREGULAR RR
	VPC
	SVPC
	RHYTHM CHG
	NEW FORM
	NEW NORMAL BEAT

Parameter	Message
SpO2	Module Failure
	Too Many Params
	Connector Off
	Probe Off
	Probe Disconnect
	Probe Broken
	No Pulse
	Light Interfer.
	Pulse Search
	Check Probe Site
	M (Unstable Pulse)
	Small Pulse
	Check Label
	Probe Off
	Probe Broken
	Hardware Control
	Noise
	Cal Start
	Cal Complete

Parameter	Message
RESP	Module Failure
	Too Many Params
	Connector Off
	Check Sensor
	Check Label
	Power Off
	Resp Off

Parameter	Message
NIBP	Module Failure
	Too Many Params
	Connector Off
	Safety Valve Open
	No pulse
	Meas Time Out
	Check Cuff/Hose
	Systolic Over
	High Cuff Pressure
	Re-measuring
	Please Wait
	Small Pulse
	Zeroing
	Noise
	Check Sensor
	Cannot Measure
	Check Cuff/Hose

Parameter	Message
PRESS	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	Out of Range
	Zero Imbalance
	Zero Unstable
	Zero Out of Range
	Zeroing Complete
	Noise

Parameter	Message
Temp	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor

Parameter	Message
CO_2	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	Line Block

Parameter	Message
FiO_2	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	Sensor Run Down?
	Cal?
	Calibration Error
	Calibrating

Parameter	Message
FLOW	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	Change Sensor
	Calibrating

Parameter	Message
$S\bar{v}O_2$	Module Failure
	Too Many Params
	Check Label
	OM2 Disconnected
	Check OM2
	OM2 Failure
	Check OM2 Light
	OM2 Error
	Out of Range
	Auto Zero
	Calibration Error

Parameter	Message
CCO	Unit Failure
	Too Many Params
	Check Label
	Connector Off
	Check Catheter
	Catheter Location
	Meas Failure
	Com Error
	Alarm
	Standby
	Tb Out of Range
	Unstable Tb
	Signal Adapting
	CO<1.0L/m

Parameter	Message
ANES	Unit Failure
	Too Many Params
	Check Label
	Illegal Module
	SAM Failure
	Moisture Detected
	Over Temp
	SAM Not Installed
	Com Error
	GAS Liquefied
	Check Sampl Line
	Blocked Sampl Line
	Install Aquaknot
	Remove Aquaknot
	Alarm
	Check
	Sensor Failure
	O2 Sensor Failure
	Calibrating(Zero)
	Warming Up
	DES??
	Standby
	Calibrating
	Calibration Error
	Apnea

Parameter	Message
tcPO2/tcPCO2	Module Failure
	Com Error
	Alarm
	ConnectorOff

Parameter	Message
BIS	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	DSC Failure
	Com Error
	Alarm
	Imp. Checking
	High Impedance

Parameter	Message
CNIBP	Unit Failure
	Connector Off
	Check Sensor
	Com Error
	Pulse Search
	Sensor Expired
	Check
	Out of Range

Parameter	Message
EEG	Module Failure
	Too Many Params
	Check Label
	Connector Off
	Check Sensor
	Alarm

Parameter	Message
VENT	Alarm

Other

Trouble	Possible Cause/Criteria	Action
SIGNAL LOSS	Weak electric field strength of a wireless telemeter.	Check the followings: • Remaining charge of the transmitter battery • Transmitter antenna lead condition • Distance between the multiple patient receiver and transmitter
BATTERY	Weak transmitter battery	Replace the batteries with new ones.
CALL	The CALL button on the transmitter was pressed.	---
MONITOR OFF	The selected bedside monitor power is OFF or is disconnected from the network.	---
	The multiple patient receiver for the transmitter is disconnected from the network.	---
OFF	The bed is discharged.	---

SIGNAL LOSS, BATTERY and CALL are displayed only when receiving data from a transmitter.

Messages From Central Monitor

WS-971R Recorder Unit

Trouble	Possible Cause/Criteria	Action
RECORDER DOOR OPEN	The recorder unit door is not closed completely.	Close the door completely.
RECORDER OUT OF PAPER	No recording paper in the recorder unit.	Set recording paper in the recorder unit. If there is recording paper in the recorder unit and the message still appears, the paper detection sensor is malfunctioning. Clean the sensor part in the recorder unit.
RECORDER POWER OFF OR DISCONNECTED	The recorder unit is disconnected.	Connect the recorder unit.
	The recorder unit is turned OFF.	Turn the recorder unit power ON.

Laser Printer

Trouble	Possible Cause/Criteria	Action
Printer is OFF LINE	The laser printer is not registered.	Contact your Nihon Kohden distributor or representative.
Printer is OUT OF PAPER	No paper in the laser printer.	Set paper in the printer. Refer to the printer manual.
Job Error	Error in the printer.	Refer to the printer manual.
Paper tray is open	The laser printer cover is not closed completely.	Close the cover completely.

Other

Trouble	Possible Cause/Criteria	Action
OFF	The bed is discharged.	---
Temporary Discharge	The bed is temporarily discharged.	To resume monitoring, touch “Resume” on the Pause window of the Admit/Discharge of the Personal Setup.

Hard Disk Replacement Flow

When you order a new hard disk for replacement, the new hard disk has the OS (Windows 2000) and central monitor system program installed at the factory. Therefore, you do not have to install these. Replace the old hard disk with the new one according to the following procedure.

1. Write down the following settings.
   - IP address of the personal computer used as the central monitor main unit.
   - The central monitor settings which are different from the factory default settings.
   - IP address of the network printer

2. Save the printer driver software on a storage media such as floppy disk or CD-R if you use a printer which is not recommended by us.

3. Replace the old hard disk with the new one according to the “Replacing the Hard Disk” in Section 4 “Disassembly and Assembly”.

4. Connect the display unit, keyboard, mouse and protection key to the central monitor main unit. Refer to “Connection Diagram of Central Monitor” in Section 1.

5. Turn on the peripheral units and main unit. The main unit automatically recognizes the hardware components. The hardware information stored in the new hard disk changes to the actual hardware information. The central monitor system program automatically runs.

6. Shut down the central monitor according to the shutdown procedure in the operator’s manual.

7. If a restart request dialog box appears on the screen, restart Windows 2000.

8. Check that there is no restart request dialog box on the screen. If the restart request dialog box is still there, repeat the restart of Windows 2000 until the restart request dialog box does not appear. The number of restart request dialog box appearances depends on the hardware composition of the central monitor.

9. Run the central monitor system program.

10. Set the IP address on the central monitor. Refer to “Setting the IP Address on Each Instrument” in Section 8 “Network Settings”.

11. Connect the central monitor to the network. Refer to “Network and System” installation guide. On the central monitor, check that each instrument is connected to the network. Refer to “Checking the Network Connection on the Central Monitor” in Section 8 “Network Settings”.

12. Install the network printer drive into the central monitor under Windows 2000. Refer to “Installing the Laser Printer (Network Printer)” in Section 8 “Network Settings”.

13. Assign the central monitor name under Windows 2000 and assign the group name under the central monitor system program if necessary. Refer to “Assigning the Group Name and Bed Name” in Section 8 “Network Settings”.

14. If some settings which are different from the factory default settings are used, change the corresponding default settings to the necessary settings at the central monitor. Refer to “Changing Setting of System Setup, Patient Setting and Setup” in Section 8 “Network Settings”.

How to Recover the BIOS Initial Settings

When the BIOS (Basic Input/Output System) settings are lost because the lithium battery on the motherboard is completely discharged, the following message appears on the screen at the beginning of the boot.

BIOS Checksum Error - Default loaded

To recover the BIOS initial settings, replace the lithium battery with a new one or press the F1 key on the keyboard each time the message appears.

If there is an electric shock such as lightning, the BIOS setting can be lost. The above message appears on the screen if the BIOS settings are lost. To recover the BIOS initial settings, press the F1 key on the keyboard.

If the BIOS settings are lost for any other reasons, perform the following procedure to recover the BIOS initial settings.

1. Connect a keyboard to the central monitor main unit.

2. Turn on the main unit. The self-check program runs.

3. Press the Delete key on the keyboard during the run of the self-check program. The BIOS setting screen appears. If the BIOS setting screen does not appear, turn off the main unit and remove the lithium battery from the motherboard. Start this procedure from step 2.

4. Select “Load Setup Defaults”.

5. Select “Save & Exit Setup” to exit the BIOS setting screen.

BIOS Default Setting (Vorax5000)

The BIOS setting may differ depending on the production lot.

Standard CMOS features	Date/Time	Current date and time
	IDE Primary Master	AUTO (Indicates the recognized hard disk model)
	IDE Primary Slave	AUTO (Indicates the recognized hard disk model)
	IDE Secondary Master	AUTO (IDE Secondary Master) AUTO (Access mode)
	IDE Secondary Slave	AUTO (IDE Secondary Master) AUTO (Access mode)
	Drive A	1.44 MB 3.5 inch
	Drive B	None
	VIDEO	EGA/VGA
	HALT On	All Errors

Advanced BIOS Features	Virus Warning	Disabled
	CPU Internal Cache	Enabled
	External Cache	Enabled
	CPU L2 Cache ECC checking	Enabled
	Processor Number Feature	Enabled
	Quick POWER ON Self test	Enabled
	First Boot Device	A:
	Second Boot Device	C:
	Third Boot Device	CDROM
	Boot Other Device	Enabled
	Swap Floppy Disk	Disabled
	Boot Up Floppy Seek	Disabled
	Boot up NumLock Status	Off
	Typematic Rate Setting	Disabled
	Security Option	Setup
	OS select for DRAM > 64MB	Non-OS2
	Show Logo On Screen	Disabled

Advanced Chipset Features	SDRAM CAS Latency Time	3
	SDRAM Cycle Time Tras/Trc	7/9
	SDRAM RAS-to CAS Delay	3
	SDRAM RAS Precharge Time	3
	SM I/O Buffer Control	Normal
	System BIOS Cashable	Disabled
	Video BIOS Cashable	Disabled
	Delayed Transaction	Enabled
	AGP MODE	AUTO

Integrated Peripherals	On-Chip Primary PCI IDE	Enabled
	On-Chip Secondary PCI IDE	Enabled
	IDE Primary Master PIO	Auto
	IDE Primary Slave PIO	Auto
	IDE Secondary Master PIO	Auto
	IDE Secondary Slave PIO	Auto
	IDE Primary Master UDMA	Auto
	IDE Primary Slave UDMA	Auto
	IDE Secondary Master UDMA	Auto
	IDE Secondary Slave UDMA	Auto
	USB Controller	Enabled
	USB Keyboard support	Disabled
	Init Display First	PCI Slot
	AC97 Audio	Auto
	OnBoard CNR LAN	Enabled
	IDE HDD Block Mode	Enabled
	POWER ON Function	Button Only
	OnBoard FDC Controller	Enabled
	OnBoard Serial Port 1	3F8/IRQ4
	OnBoard Serial Port 2	2F8/IRQ3
	UART Mode Select	Normal
	Onboard Parallel Port	378/IRQ7
	Parallel Port Mode	SPP
	AC PWR Auto Recovery	Former Status
	Game Port Address	201
	Midi Port Address	330
	Midi Port IRQ	5

Power Management Setup	ACPI Function	Enabled
	ACPI Suspend Type	S1
	Power Management	User Define
	Video Off Method	V/H SYNC + Blank
	Video Off In Suspend	Yes
	Suspended Type	CPU Sleep Mode
	Modem Use IRQ	3
	Suspend Mode	Disabled
	HDD Power Down	Disabled
	Soft Off by Power Button	Instant Off
	Wake On PCI Card	By OS
	Wake On Modem	Disabled
	Wake On LAN	Disabled
	Wake On RTC	By OS
	Primary IDE 0	Disabled
	Primary IDE 1	Disabled
	Secondary IDE 0	Disabled
	Secondary IDE 1	Disabled
	FDD, COM, LPT Port	Disabled
	PCI PIRQ [A-D]#	Disabled

PnP Configurations	Reset Configuration Data	Disable
	Resources Controlled by	Auto (ESCD)
	PCI/VGA Palette Snoop	Disabled
	Assign IRQ For VGA	Enable
	Assign IRQ For USB	Enable

PC Health Status	Shut down Temperature	Disabled

PASSWORD	-	None

BIOS Default Setting (Vorax5001)

The BIOS setting may differ depending on the production lot.

Standard CMOS features	Date/Time	Current date and time
	IDE Primary Master	AUTO (Indicates the recognized hard disk model)
	IDE Primary Slave	AUTO (Indicates the recognized hard disk model)
	IDE Secondary Master	AUTO (IDE secondary Master) AUTO (Access mode)
	IDE Secondary Slave	AUTO (IDE Secondary slave) AUTO (Access mode)
	Drive A	1.44 MB 3.5 inch
	Drive B	None
	VIDEO	EGA/VGA
	HALT On	All Errors

Advanced BIOS Features	Virus Warning	Disabled
	CPU L1 & L2 Cache	Enabled
	Quick POWER ON Self Test	Enabled
	First Boot Device	A:
	Second Boot Device	C:
	Third Boot Device	CDROM
	Boot Other Device	Enabled
	Swap Floppy Disk	Disabled
	Boot Up Floppy Seek	Disabled
	Boot up NumLock Status	ON
	Gate A20 Option	Normal
	TypeMedia Rate Setting	Disabled
	Security Option	Setup
	APIC Mode	Enabled
	Report No FDD for WIN 95	No
	Show Logo On Screen	Disabled

Advanced Chipset Features	Dram Read Thermal Mgmt	Disabled
	System BIOS Cacheable	Disabled
	Video BIOS Cacheable	Disabled
	Video RAM Cacheable	Disabled
	Memory Hole At 15M-16M	Disabled
	Delayed Transaction	Enabled
	CPU Auto Throttling Delay	16Min
	AGP Aperture Size (MB)	64

Integrated Peripherals	On-Chip Primary PCI IDE	Enabled
	IDE Primary Master PIO	Auto
	IDE Primary Slave PIO	Auto
	IDE Primary Master UDMA	Auto
	IDE Primary Slave UDMA	Auto
	On-Chip Secondary PCI IDE	Enabled
	IDE Secondary Master PIO	Auto
	IDE Secondary Slave PIO	Auto
	IDE Secondary Master UDMA	Auto
	IDE Secondary Slave UDMA	Auto
	USB Controller	Enabled
	USB Keyboard support	Disabled
	USB Mouse Support	Disabled
	AC97 AUDIO	Auto
	AC97 MODEM	Auto
	Init Display First	PCI Slot
	OnBoard LAN Conroller	Enabled
	IDE HDD Block Mode	Enabled
	POWER ON Function	Button Only
	Onboard FDC Controller	Enabled
	Onboard Serial Port 1	3F8/IRQ4
	Onboard Serial Port 2	2F8/IRQ3
	UART Mode Select	Normal
	Onboard Parallel Port	378/IRQ7
	Parallel Port Mode	SPP
	PWRON After PWR-fail	Former-sts
	Game Port Address	201
	Midi Port Address	330
	Midi port IRQ	10
	Case Opened Warning	Disabled

Power Management Setup	ACPI Suspend Type	S1 (POS)
	Power Management	User Define
	Video Off Method	V/H SYNC + Blank
	Video Off In Suspend	Yes
	Suspended Type	Stop Grant
	Modem Use IRQ	3
	Suspend mode	Disabled
	HDD Power Down	Disabled
	Soft-Off by PWR-BTTN	Instant-Off
	Wake-Up By PCI Card	Disabled
	Power On By Ring	Disabled
	Resume By Alarm	Disabled
	Primary IDE 0	Disabled
	Primary IDE 1	Disabled
	Secondary IDE 0	Disabled
	Secondary IDE 1	Disabled
	FDD, COM, LPT Port	Disabled
	PCI PIRQ [A-D]	Disabled

PnP/PCI Configuration	Reset Configuration Data	Disabled
	Resources Controlled By	Auto (ESCD)
	PCI/VGA Palette Snoop	Disabled

PC Health Status	Shutdown Temperature	Disabled

CPU/PCI Clock Control	Spread Spectrum	Disabled
	Fixed AGP/PCI Freq.	Disabled
	CPU Clock	133
	Memory Frequency For	Auto
	DRAM Timing Selectable	Manual
	CAS Latency Time	2.5
	Active to Precharge Delay	6
	DRAM RAS# to CAS# Delay	3
	DRAM RAS# Precharge	3

PASSWORD	-	None

Section 3 Board/Unit Description

Power Supply Unit (by NIPRON) 3.1
Motherboard (by A-OPEN) 3.1
CPU (1 GHz Pentium 3 or 2.4 GHz Pentium 4) Box 3.1
256 MB Memory DIMM S-DRAM or DDR266 ..... 3.2
40 GB Hard Disk (by IBM) 3.2
CD-ROM Drive (by SAMSUNG) 3.2
Graphic Board RADEON 32 or RADEON 7000 (by ATI) 3.2
PC Chassis IW-V500 or IW-V500G 3.3
Fan for Chassis 3.3
Mouse 3.3
RS232C Interface Board CYBER SERIAL 3.3

This page is intentionally left blank.

Power Supply Unit (by NIPRON)

The power supply unit accepts AC line voltages of 100 to 240 V AC. The fan in the power supply unit automatically changes the rotation speed according to the temperature of the power supply unit.

Motherboard (by A-OPEN)

The motherboard has the following functions.

- CPU socket for the CPU (1 GHz Pentium 3 or 2.4 GHz Pentium 4) chip
- Floppy disk drive interface
- ATA/66M interface for hard disk drive
- Ethernet interface
- Sound drive circuit
- RS232C serial data interface (2 ports provided)
- Parallel data interface
- PCI bus (3 PCI sockets provided)
- AGP bus (Not used)
- Game control interface (Not used)
- USB interface (Not used)

Since each component on the motherboard is individually checked in the aging test at the manufacturer, the motherboard has higher reliability than the commercially available same model.

CPU (1 GHz Pentium 3 or 2.4 GHz Pentium 4) Box

This box consists of the CPU chip and fan for the CPU.

256 MB Memory DIMM S-DRAM or DDR266

One chip 256 MB memory for working area is used. In future, a compatible memory which has more working area may be used.

40 GB Hard Disk (by IBM)

An IBM hard disk with IDE interface is used. A compatible hard disk which has more data storage may replace the current hard disk in future.

CD-ROM Drive (by SAMSUNG)

A CD-ROM drive with IDE interface is used.

Graphic Board RADEON 32 or RADEON 7000 (by ATI)

The graphic board has a PCI interface. Two same graphic boards are installed in the main unit so that they allow you to use the two displays in dual mode.

If one of the two boards has a failure, the other board can be used for the display unit of the central monitor. To use the board, assign the board as “1” in screen properties in Windows 2000. Only the RADEON 32 (for Vorax5000) and RADEON 7000 (for Vorax5001) graphic boards are compatible because the CNS system program was designed for these graphic boards only.

PC Chassis IW-V500 or IW-V500G

The front panel, right and left side panels and top cover are included in the chassis. Note that the labels on these panels are not included in the chassis.

Fan for Chassis

A silent type fan is used. The size is 80 mm square. The current fan may be replaced with a compatible one in future.

Mouse

A Microsoft PS-2 mouse is used. If you use a third party mouse of lower quality, the mouse may cause a problem. Therefore, use the recommended mouse.

RS232C Interface Board CYBER SERIAL

There are two serial data communication ports on the board. The board has a PCI interface and is used for the serial data communication with the touch screen. If this board or touch screen has a failure, you can work the central monitor using the mouse and keyboard without the touch screen function.

This page is intentionally left blank.

Section 4 Disassembly and Assembly

Before You Begin 4.1
- Warnings and Caution 4.1
- Required Tools 4.1

Disassembling the Main Unit 4.2
- Replacing the Motherboard 4.2
- Replacing the Lithium Battery on the Motherboard 4.10
- Replacing the CPU 4.10
- Replacing the Internal Memory 4.10
- Replacing the Hard Disk 4.11
- Replacing the Graphic Board 4.11
- Replacing the Fans 4.11
- Replacing the Floppy Disk Drive 4.12
- Replacing the Power Supply Unit 4.12
- Replacing the CD Drive 4.12

Disassembling the Optional VL-971R Display Unit 4.13
- Replacing the LCD Assembly 4.13
- Removing the Display Unit Chassis 4.15
- Replacing the Touch Screen 4.19

Disassembling the Optional WS-971R Recorder Unit 4.20
- Removing the Recorder Sub Assy 4.20
- Removing the AC Inlet Socket 4.21
- Removing the RS232C Interface Board 4.22
- Removing the Power Supply Unit 4.22
- Removing the Front Panel 4.22
- Replacing the LED 4.23
- Replacing the Platen Roller/Bushings/Gear 4.24
- Cleaning the Thermal Array Head/Paper Sensor 4.25
- Operation Check after Assembling the Recorder Unit 4.25

This page is intentionally left blank.

The procedures in this section tell how to remove, replace and install the major components in the instrument.

Before You Begin

Removing, replacing and installing the major components should be done by qualified service personnel.

Warnings and Caution

WARNING

- **To avoid the possibility of injury to yourself or damage to the instrument, do not install or remove any component or change the internal switch settings while the power is on. After the power is off, wait a few minutes before disassembling the instrument.**
- **To avoid accidental discharge of static electricity, which could damage the instrument components, use a wrist ground strap when installing or removing any component.**

CAUTION

Fuses cut off the power when an abnormality occurs in the instrument. Eliminate the malfunction before replacing the fuse. Use the correct fuse only. The fuse rating is shown on the holder.

Required Tools

Anti-static bench mat
Anti-static wrist strap
Flat-blade screwdriver (insulated type)
Phillips screwdriver (insulated type)
Allen wrench or hexagon keys
Hex socket driver
Tweezers
Nippers
Cable tie

Disassembling the Main Unit

Before performing the following procedure, shut down the main unit according to the operator's manual and disconnect the power cord from the main unit.

Replacing the Motherboard

1. <Vorax5000>

   Remove the 2 screws which secure the side panel to the main unit. Remove the side panel from the main unit.

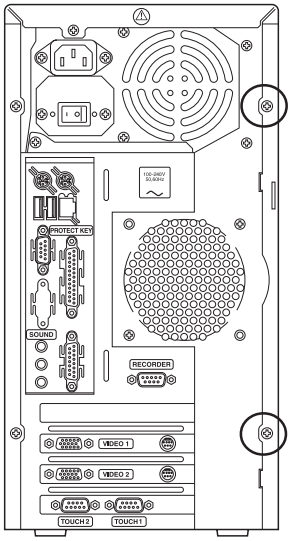

<Vorax5001>

Remove the 2 screws which secure the side panel to the main unit.

Release the 2 hooks which secure the side panel to the main unit by pulling the hooks outward, as shown by the arrows in the following figure. Remove the side panel from the main unit.

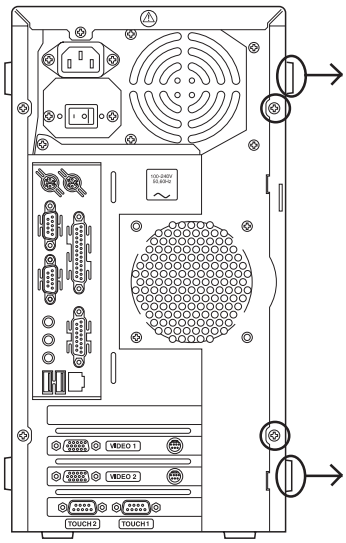

NOTE in Assembling the Main Unit

To attach the side panel to the main unit, put the lower edge of the side panel into the guide rail of the main unit chassis.

2. Remove the 3 screws which secure the 2 graphic boards and serial interface board to the chassis. Remove the 3 boards from the main unit.

3. Remove the screw which secures the disk case to the chassis as shown below.

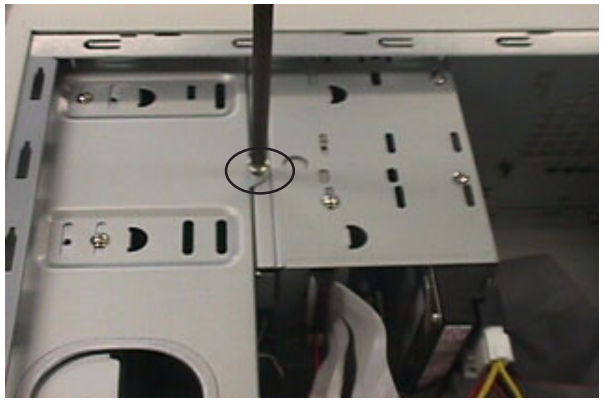

4. Disconnect the flat cable between the hard disk and motherboard. At the motherboard, disconnect the floppy disk drive flat cable.

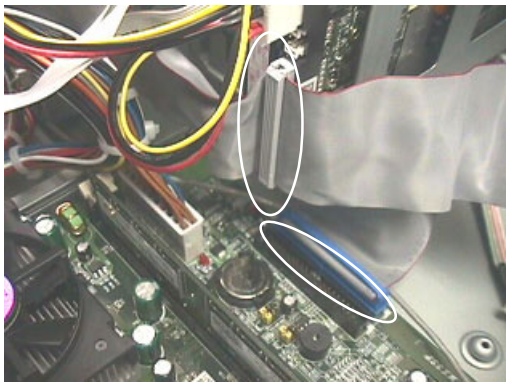

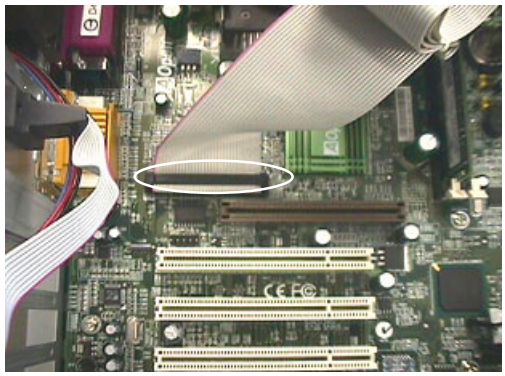

CAUTION

If disconnecting the flat cable at the floppy disk drive, note the flat cable connector direction because the connector has no mechanism to prevent wrong connection.
If you forget the connector direction, align the pink line of the flat cable and the pin No. 1 of the socket.

NOTE in Assembling the Main Unit

Connect the blue connector of the hard disk flat cable to the IDE1 socket on the motherboard.

5. Disconnect each power supply cable from the hard disk and floppy disk drive.

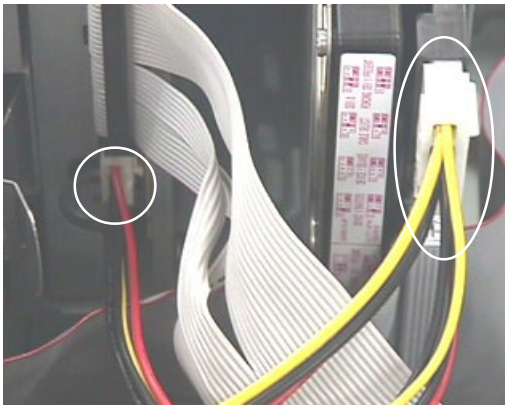

6. Remove the disk case from the main unit by pulling the hook of the disk case and sliding the hook rearward as shown below.

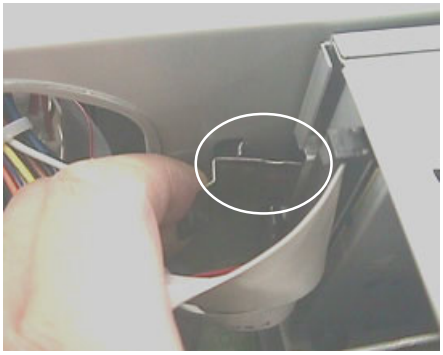

NOTE in Assembling the Main Unit

To attach the disk case to the main unit, continue pulling the hook and slide it in the hole of the chassis frontward until the hook clicks.

7. Disconnect the power supply cable from the motherboard.

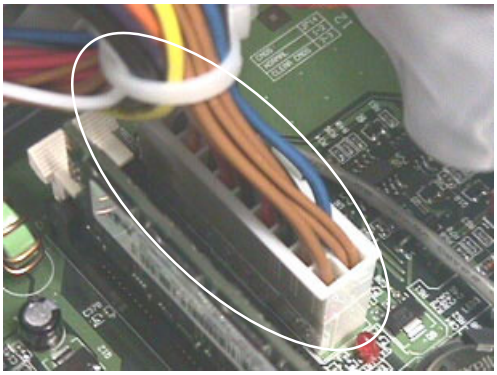

8. Disconnect the connection cable from the front panel which has the power switch, power indicator, hard disk operation indicator and reset switch.

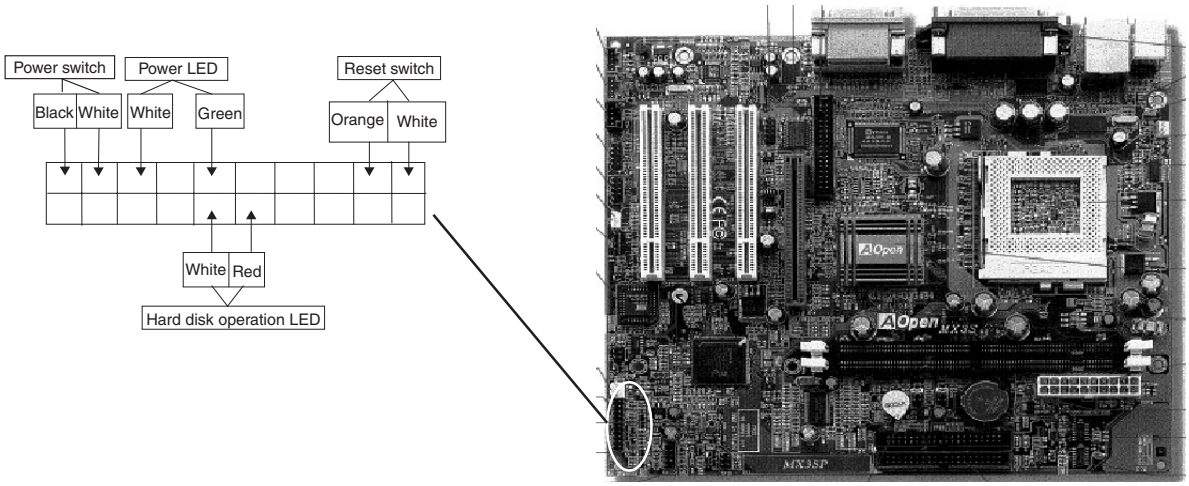

9. Disconnect the following cables from the motherboard.
   - CD-IN cable which connects to the CD drive.
   - FAN1 cable which connects to the fan on the rear panel.
   - COM2 black cable which connects to the RECORDER socket (COM2 port) on the rear panel.

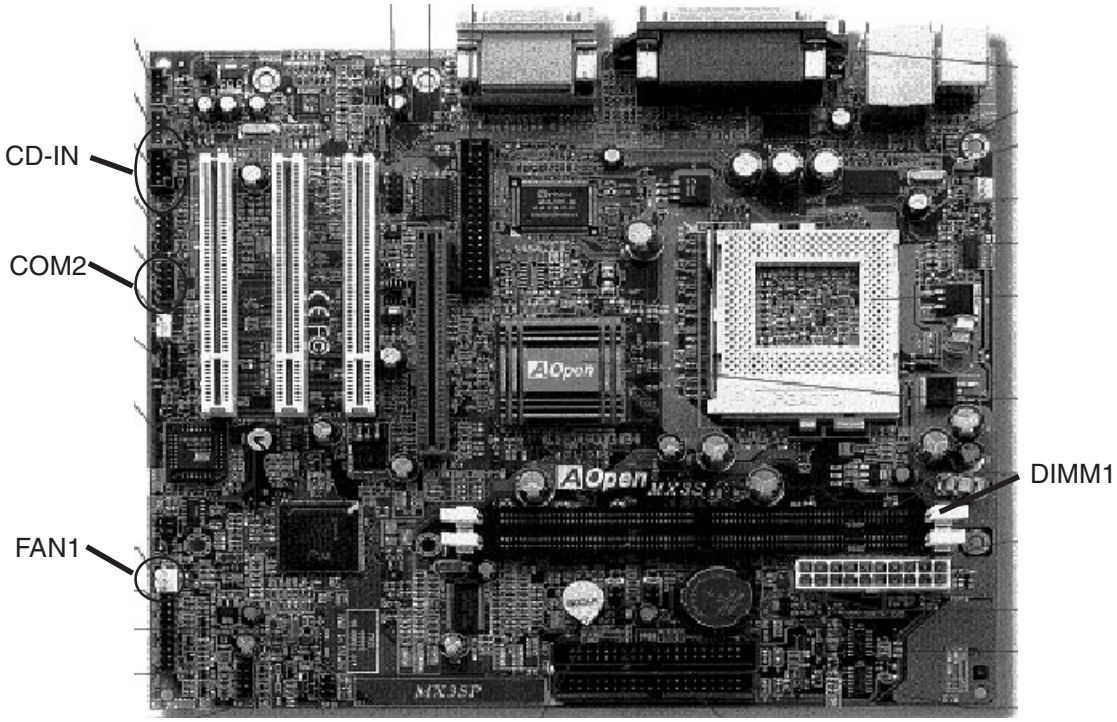

NOTE in Assembling the Main Unit

To connect a flat cable to the motherboard, align the pink line of the flat cable and the pin No. 1 of the socket.

10. Remove the 6 screws which secure the motherboard to the chassis. Remove the motherboard from the main unit.

NOTE in Assembling the Main Unit

To attach the motherboard to the main unit, tighten the 6 screws while pushing the motherboard to the rear panel until the 6 holes of the motherboard match the screw holes of the chassis.

11. Depress the white hooks which fasten the DIMM board to the socket. Remove the DIMM board from the motherboard.

NOTE in Assembling the Main Unit

To attach the DIMM board to the motherboard, insert the DIMM board into the DIMM1 socket on the motherboard. Latch the DIMM board with the hooks.

<Vorax5000> When the main unit is Vorax5001, go to step 12 of <Vorax5001>.

12. Disconnect the brown connector of the CPU fan cable from the motherboard.

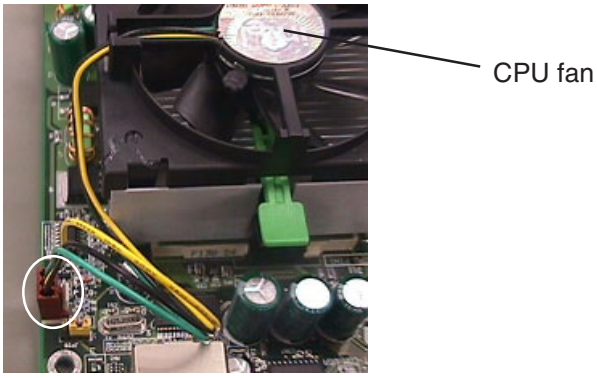

13. Release the 4 hooks of the CPU fan as shown below by inserting a small flat-blade screwdriver between the longer hook of the CPU fan and heat sink. Remove the CPU fan from the motherboard.

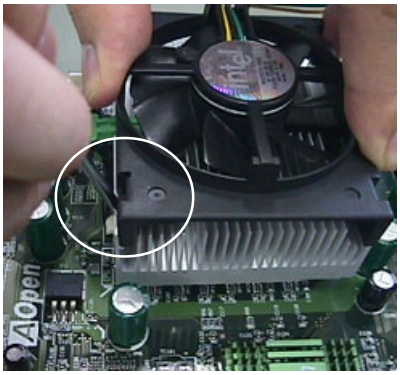

NOTE in Assembling the Main Unit

To attach the CPU fan to the motherboard, latch the 2 short hooks of the CPU fan on the heat sink and press the other 2 long hooks of the CPU fan to the heat sink.

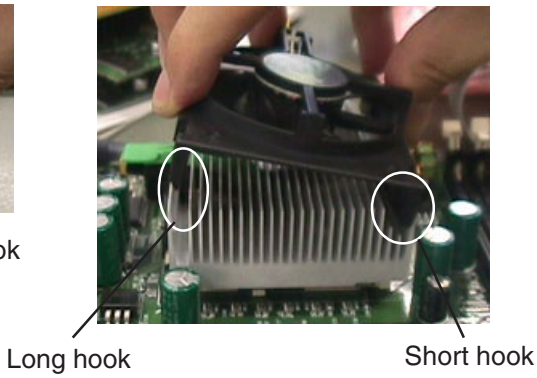

14. Pull up the green lever for fastening the heat sink. Insert a small flat-blade screwdriver between hook 2 of the green lever and the CPU socket and release the hook by rotating the screwdriver. Remove the heat sink from the motherboard.

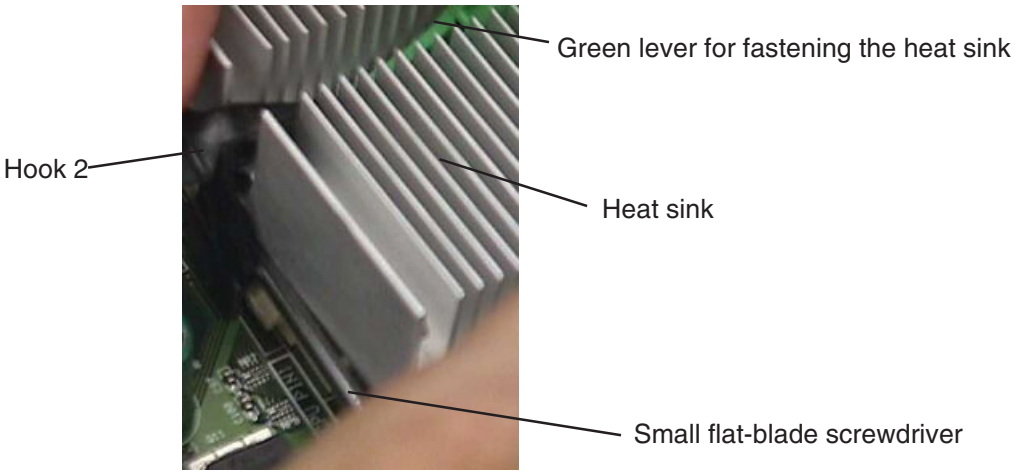

NOTE in Assembling the Main Unit

To attach the heat sink to the CPU socket lever, put the heat sink on the CPU and latch the hook 1 on the heat sink and press the hook 2 on the heat sink until the hook 2 clicks, or put the heat sink on the CPU and latch the hooks 1 and 2 on the CPU socket. Put the green lever back to the original position.

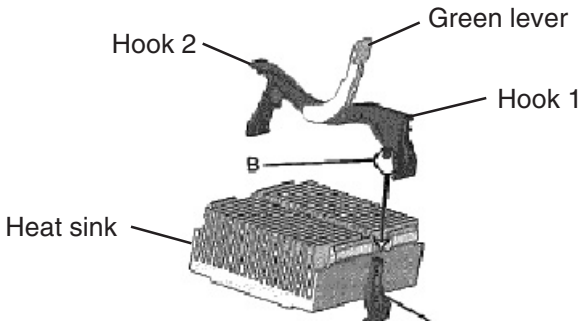

15. Pull the lever of the CPU socket upward and remove the CPU from the motherboard.

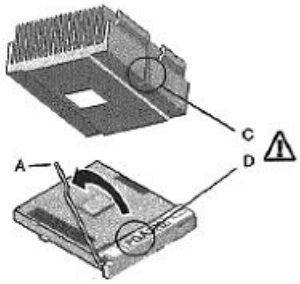

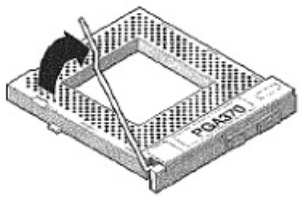

NOTE in Assembling the Main Unit

To attach the CPU to a new motherboard, check the correct direction of the CPU as shown below.



16. Replace the motherboard with a new one. Check that the new motherboard has the same jumper settings as the old one as shown below. Assemble the main unit by reversing the above procedure. Turn on the main unit and check the operation using the display unit connected to the main unit.
    JP14: Short-circuit between pins 1 and 2
    JP23: Short-circuit between pins 1 and 2
    JP28: Short-circuit between pins 1 and 2
    JP29: Short-circuit between pins 1 and 2

<Vorax5001>

12. Disconnect the CPU fan cable from the motherboard.

13. Release the 4 hooks of the CPU fan by pulling the 2 levers near the CPU fan upward. Remove the CPU fan and heat sink from the motherboard.

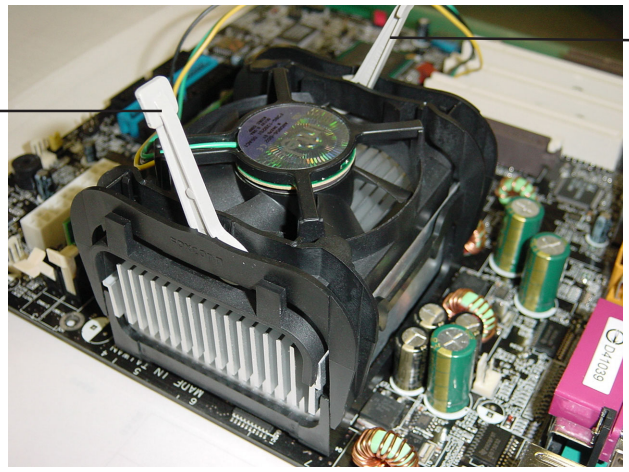

NOTE in Assembling the Main Unit

To attach the CPU fan to the motherboard, check the following.

- **Appropriate volume of silicone grease is on the bottom of the heat sink which faces the top of the CPU.**
- **The 2 levers near the CPU fan are pulled upward.**

Latch the 4 hooks of the CPU fan on each catch of the lower housing for the CPU fan and heat sink, and put the 2 levers back to the original position.

14. Pull the lever of the CPU socket upward as shown below and remove the CPU from the motherboard.

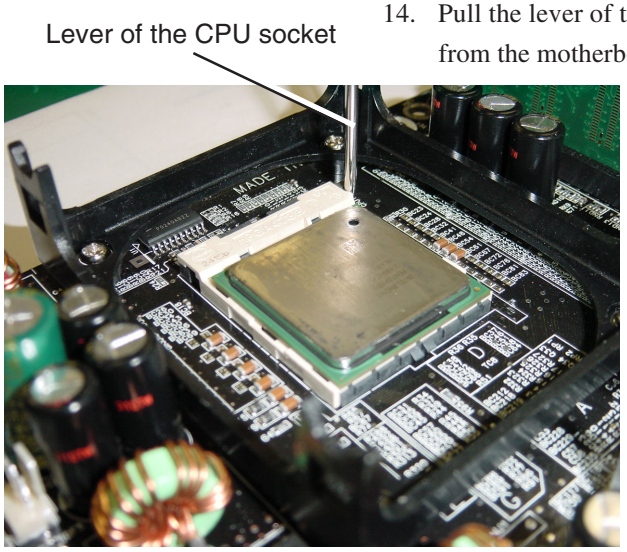

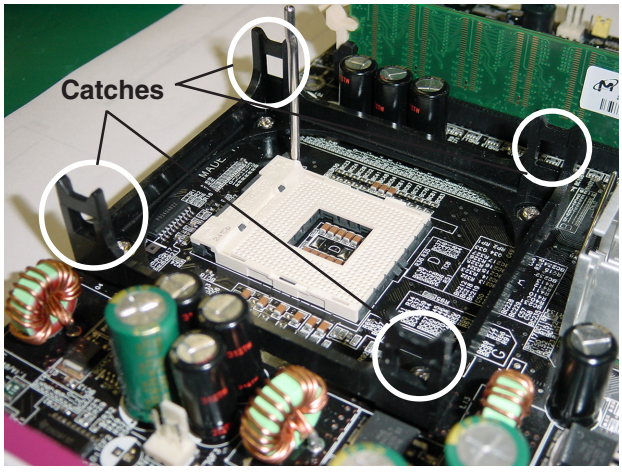

NOTE in Assembling the Main Unit

- **To attach the CPU to a new motherboard, check the correct direction of the CPU and check that the lever of the CPU socket is pulled upward.**
- **After checking that the CPU is correctly inserted into the CPU socket, put the lever back to the original position.**

15. Replace the motherboard with a new one. Check that the new motherboard has the same jumper settings as the old one. Assemble the main unit by reversing the above procedure. Turn on the main unit and check the operation using the display unit connected to the main unit.

Replacing the Lithium Battery on the Motherboard

After removing the motherboard from the main unit according to the “Replacing the Motherboard” section, replace the lithium battery with a new one.

CR-2032 Lithium Battery (3 V): 372321A

This battery allows the memory for the BIOS setting to keep the setting data and allows the real time clock IC to update the date and time while the main unit is turned off.

If the battery is used up and the main unit is completely turned off with the main power switch set to off or with the power cord disconnected, the BIOS setting data in the memory is lost and the date and time are reset to the initial condition. To recover the BIOS initial setting data, refer to “How to Recover the BIOS Initial Setting” in Section 2.

Replacing the CPU

After removing the motherboard from the main unit according to the “Replacing the Motherboard” section, replace the CPU with a new one. Refer to <Vorax5000> steps 12 to 15 or <Vorax5001> steps 12 to 14 of the “Replacing the Motherboard” section.

Replacing the Internal Memory

After removing the motherboard from the main unit according to the “Replacing the Motherboard” section, replace the internal memory with a new one. Refer to step 11 of the “Replacing the Motherboard” section.
About the internal memory of the Vorax5001 main unit, the following procedure is required after the replacement.

1. Put the motherboard back to the original position and check that the main power switch on the rear panel of the main unit is set to off and the power supply cable is not connected to the motherboard.

2. Remove the JP14 jumper attached to pins 1 and 2 on the motherboard.

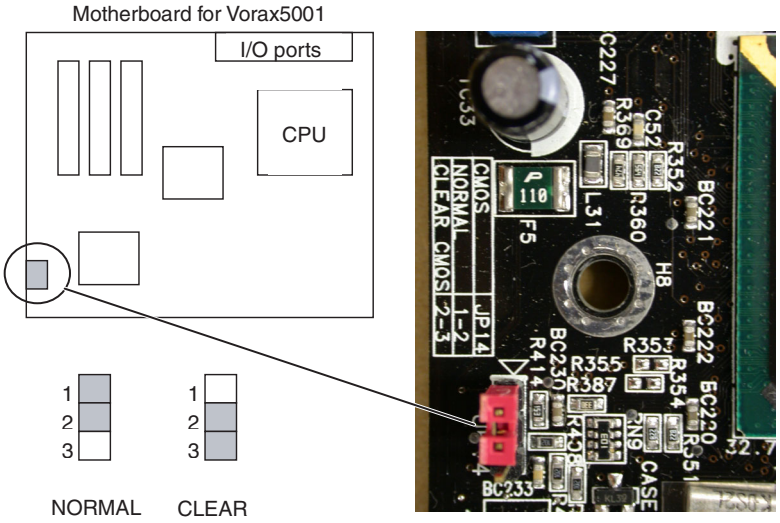

3. Attach the JP14 jumper to pins 2 and 3 on the motherboard. Wait approx. 30 seconds to initialize the BIOS settings.

4. Put the JP14 jumper back to the original position (pins 1 and 2). Connect the power supply cable to the motherboard and assemble the main unit.

5. Turn on the main unit and display unit. The self-check program runs. Press the Delete key on the keyboard while the self-check program is running. The BIOS setting screen appears.

6. Set the BIOS settings according to the "BIOS Default Setting (Vorax5001)" list in "How to Recover the BIOS Initial Settings" in Section 2 "Troubleshooting".

Replacing the Hard Disk

Before disassembling the main unit to replace the hard disk with a new one, perform the procedure described in "Hard Disk Replacement Flow" in Section 2.

1. After removing the disk case from the main unit according to the "Replacing the Motherboard" steps 1 to 6, remove the 4 screws which secure the hard disk to the disk case. Replace the hard disk with a new one.

2. Check that the jumper setting of the new hard disk is shown below. This setting which shows "Device0 (Master) in the IBM hard disk IC35L040AVER07 is the factory default setting. Windows2000 and CNS system software are installed in the hard disk at the factory.

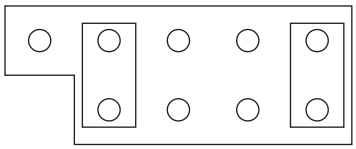

3. Assemble the main unit by reversing the above procedure.

Replacing the Graphic Board

Replace the graphic board with a new one. Refer to "Replacing the Motheboard steps 1 and 2.
Note that you can use another graphic board to temporarily solve the display problem until the new board arrives because there are two of the same graphic boards in the main unit.

Replacing the Fans

There are five fans in the main unit.

- Fan attached on the rear panel
Remove the 2 screws which secure the fan to the rear panel and replace the fan with a new one.

- Fan attached inside the power supply unit
The fan in the power supply unit is not replaceable. A fan failure requires replacement of the power supply unit. Refer to "Replacing the Power Supply Unit" section.

- Fan attached to the CPU on the motherboard
Replace the fan with a new one according to "Replacing the Motherboard".

- Fan attached to the video IC on the graphic board

Remove the graphic board from the main unit according to "Replacing the Motherboard" steps 1 to 2. Remove the screw which secures the fan to the heat sink for video IC and replace the fan with a new one.

Replacing the Floppy Disk Drive

Remove the screw which secures the drive to the disk case and replace the the drive with a new one. When attaching the disk case to the chassis after the replacement, match the drive opening and front panel opening.

NOTE in Assembling the Main Unit

To mount the floppy disk drive to the disk case, use hole No. 3 of the disk case.

Replacing the Power Supply Unit

1. Remove the 5 screws which secure the both side panels and top panel to the chassis. Remove the both side panels and top panel from the main unit.

2. Disconnect all the power supply cables from the power supply unit. When assembling the main unit after replacing the power supply unit, refer to the "Replacing the Motherboard" section.

3. Remove the 3 screws which secure the power supply unit to the rear panel and replace the power supply unit with a new one. Assemble the main unit by reversing the above procedure.

Replacing the CD Drive

1. Remove the 4 screws which secure both side panels to the chassis. Remove both side panels from the main unit.

2. Disconnect the following 3 cables from the CD drive.
   - Hard disk flat cable (for IDE connection) connected to the motherboard
   - Power supply cable (4 wires) connected to the power supply unit
   - CD-audio cable (3 wires) connected to the motherboard

3. Remove the 4 screws which secure the CD drive to the chassis and replace the CD drive with a new one. Assemble the main unit by reversing the above procedure.

Disassembling the Optional VL-971R Display Unit

To disassemble the display unit, the following tools are necessary.

- Phillips screwdriver for 3 mm in dia. screw
- Phillips screwdriver for 4 mm in dia. screw
- Hex socket driver for 1/4 inch (6.2 mm) nut

Replacing the LCD Assembly

1. Put the display unit face down on a table. The table must be covered with a clean, soft and smooth cloth to avoid damaging or making the screen dirty.
2. Remove the 12 screws (3 mm in dia.) which secure the rear cover to the front cover.

3. Turn the display unit face up on the table. Carefully separate the front cover from the display unit with the touch screen flat cable connected to the display unit.

CAUTION

If a stress is given to the touch screen flat cable, the flat cable can be easily damaged. If the flat cable is damaged, the touch screen must be replaced with a new one.

4. Remove the 12 nuts which secure the LCD assembly to the display unit chassis.

5. Slightly pull the LCD assembly upward and disconnect the digital RGB flat cable and power supply cable at the LCD assembly. Remove the LCD assembly from the display unit. The LCD assembly contains the LCD, backlight lamp and inverter for backlight lamp. These parts cannot be replaced individually. The entire LCD assembly is the minimum replaceable unit.

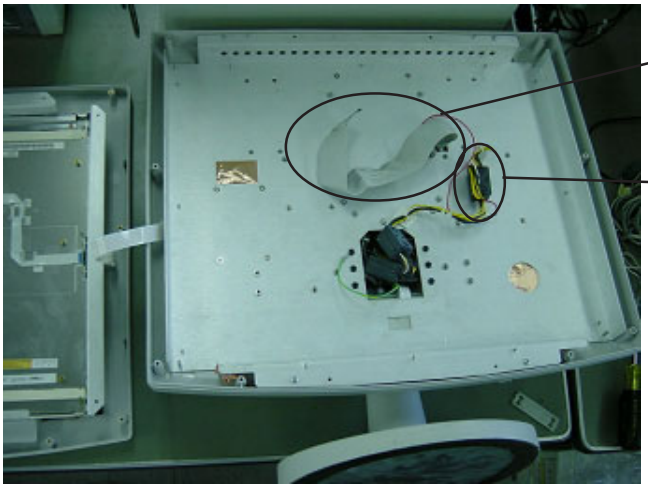

NOTE in Assembling the Display Unit

To connect the digital RGB flat cable to the LCD assembly, align the pink line of the flat cable and pin No. 1 of the socket on the LCD assembly.

Removing the Display Unit Chassis

6. Remove the 4 screws (3 mm in dia.) and 6 screws (4 mm in dia.) which secure the chassis to the rear cover.

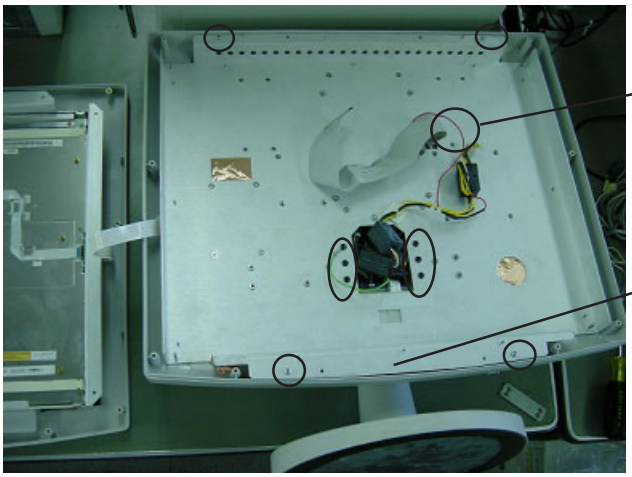

CAUTION

If the display unit has a separate wire from the power supply cable for the inverter, cut the wire to separate the chassis from the rear cover. When assembling the display unit, solder the cut wire together.

7. Pull the lower edge of the chassis upward until you can disconnect the cables from the boards on the chassis backside. Disconnect all cables from the boards and remove the chassis from the display unit.

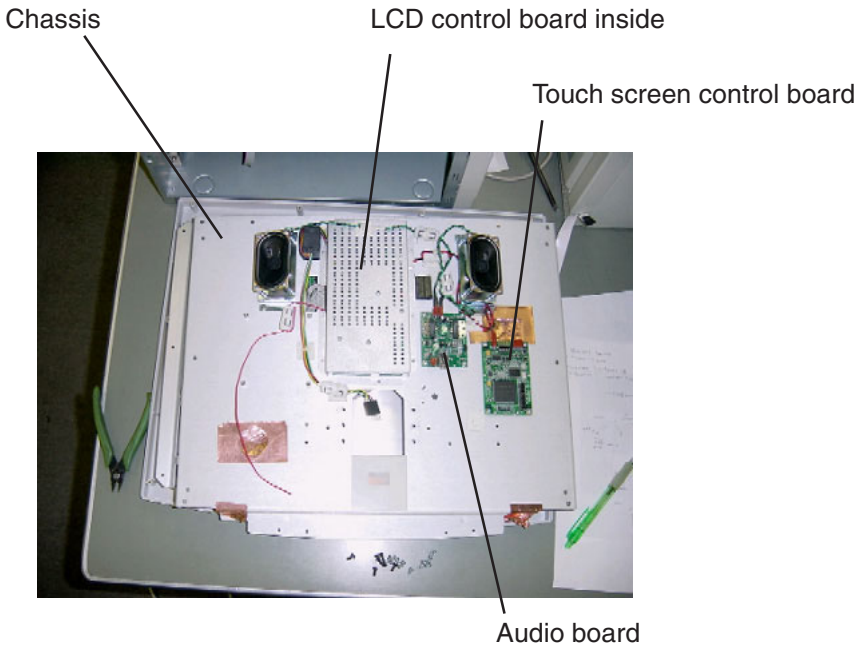

<Backside of chassis>

The following picture shows the cables which must be connected to the corresponding boards or assembly when you assemble the display unit. Refer to the cable list and partial connection diagram as shown below.

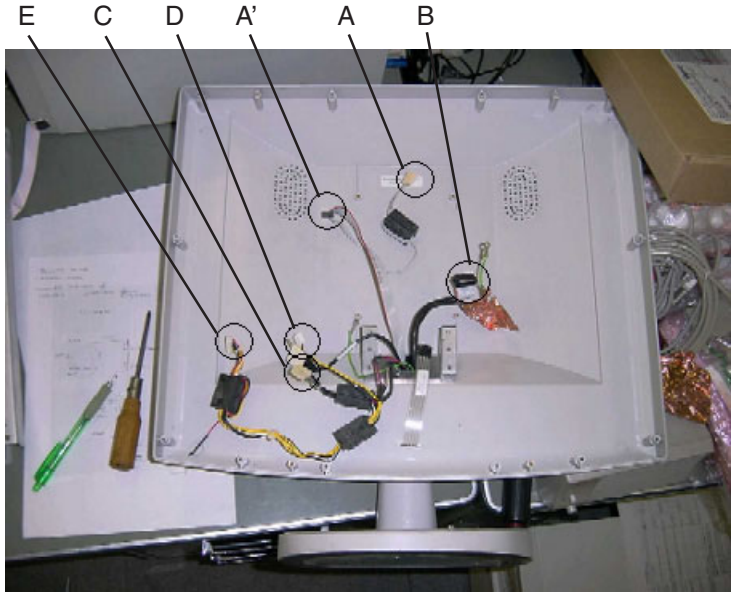

Index	Signal	Cable	Board/assembly to be connected
A	RS-232C	Flat cable, 4 wires	LCD control board
A'	RS-232C	Flat cable, 10 wires	Touch screen control board
B	Analog RGB	Flat cable, 16 wires	LCD control board
C	Supply voltages	4 wires	LCD control board
D	Supply voltages and sound signals	3 wires for power supply 4 wires for sound signals	Audio board
E	Supply voltages for inverter	? wires	LCD assembly
F	Supply voltages for touch screen control board	4 wires to 2 wires	From LCD control board to touch screen control board
G	Left audio signal	2 wires	From audio board to speaker (left)
H	Right audio signal	2 wires	From audio board to speaker (right)
I	Digital RGB	30 wires	LCD control board
J	Key status signals	5 wires	From key switch assembly to LCD control board
K	Touch screen signals	Flat cable, 5 wires	Touch screen control board

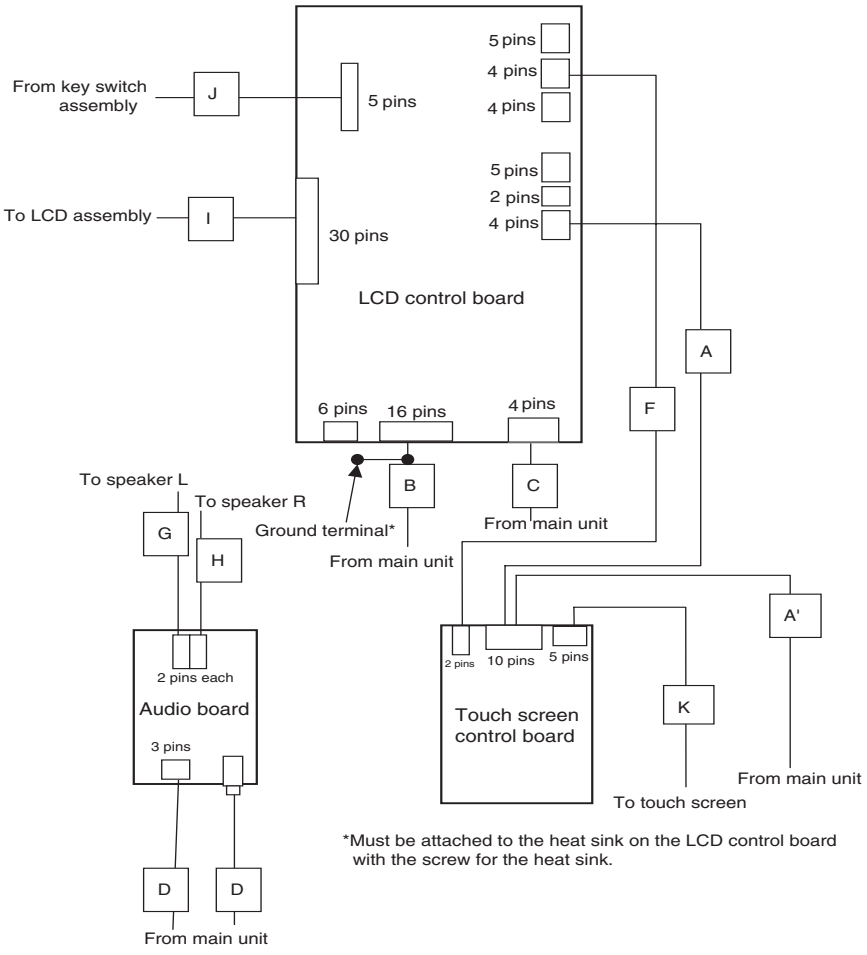

CAUTION in Assembling the Display Unit

Check that the following three things are performed when assembling the display unit.

- **Touch screen flat cable**

To connect the touch screen flat cable to the touch screen control board, align the red line of the flat cable and the pin No. 1 of the socket on the board.

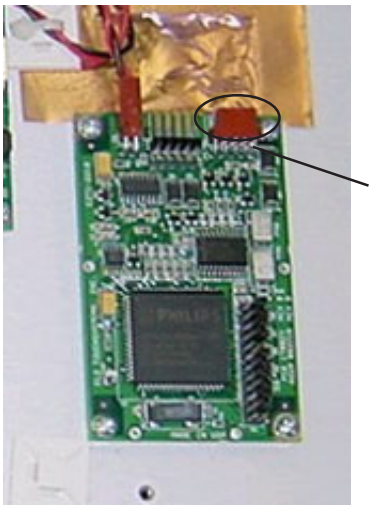

- **Connection cable between the LCD control board and key switch assembly on the rear cover**

To connect the connection cable to the LCD control board, pass the connection cable through the shield case and connect the cable to the board as shown below.

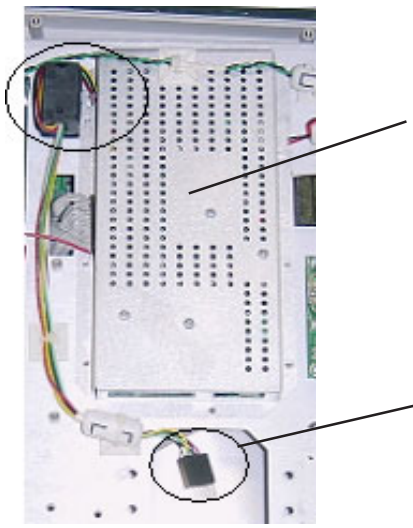

To connect the connection cable to the cable of the key switch assembly, align the connectors' pin No. 1 which is printed on the connectors. After connecting the connectors, cover the connectors with a heat shrink tube or insulation tape.

- **Ground wire from the base**

A ground wire (green/yellow) which comes from the base must be connected to the chassis with the screw (4 mm in dia.) as shown below.

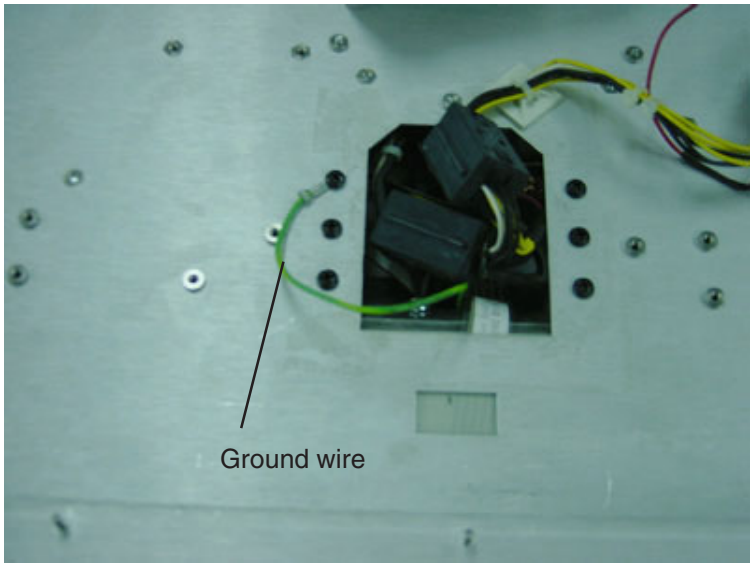

8. Replace the boards or speakers if necessary. Refer to the following connection diagram.
9. Assemble the display unit by reversing the above procedure.

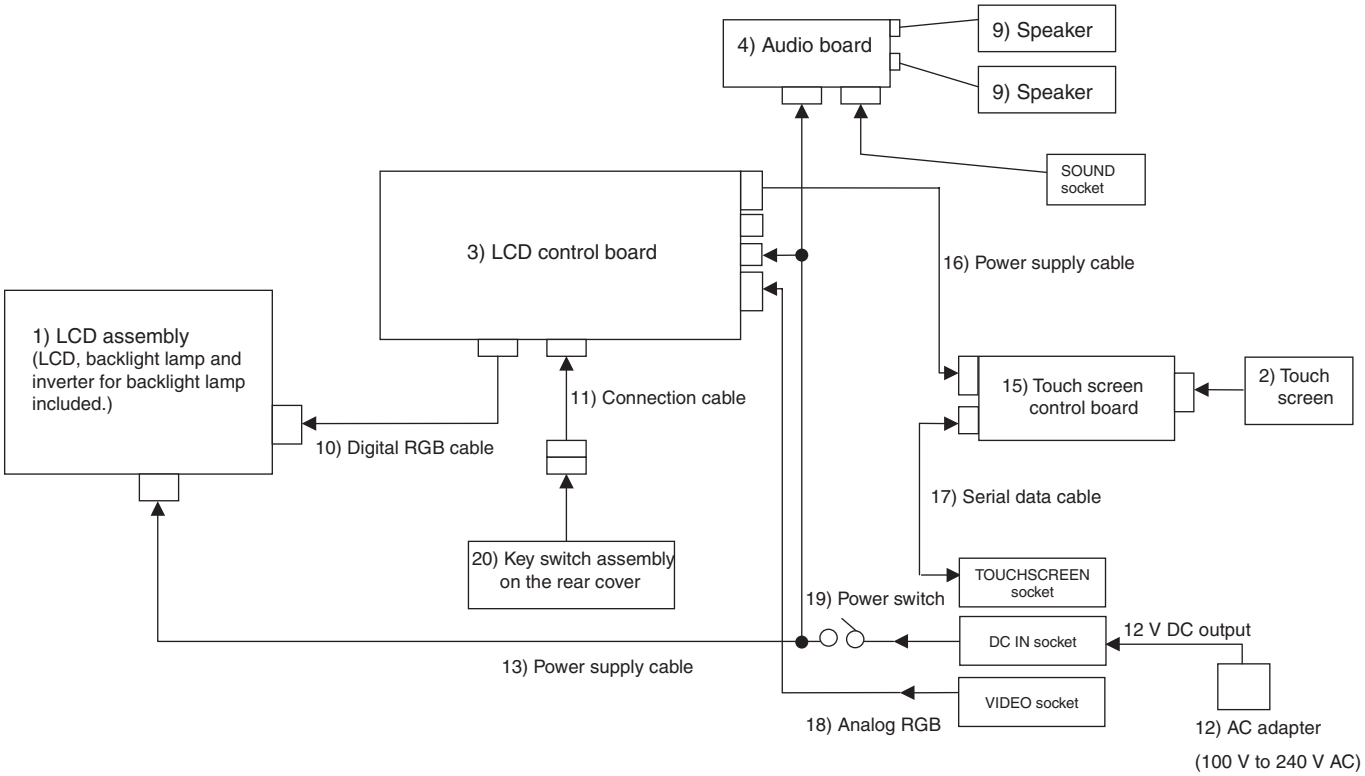

Replacing the Touch Screen

When replacing the touch screen with a new one, the following parts should also be replaced with new ones.

- Front cover: 1 pc.
- Plastic bracket for positioning of touch screen: 4 pcs.

1. Glue the 4 plastic brackets on the front cover to properly position the touch screen on the front cover.
2. Attach the touch screen to the front cover with two-sided tape* so that the touch screen is surrounded by the 4 brackets as shown below.
   *3M™ Double Coated Urethane Foam Tape 4052 is recommended.

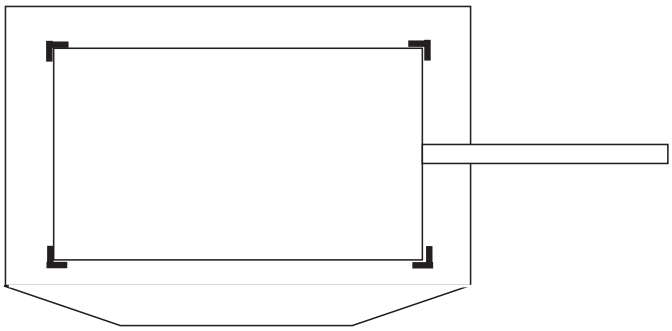

3. Put the assembled front cover back to the original position. Refer to “Replacing the LCD Assembly” steps 1 to 3.

Disassembling the Optional WS-971R Recorder Unit

Removing the Recorder Sub Assy

1. Remove the 4 screws which secure the rubber feet to the bottom of the recorder unit.

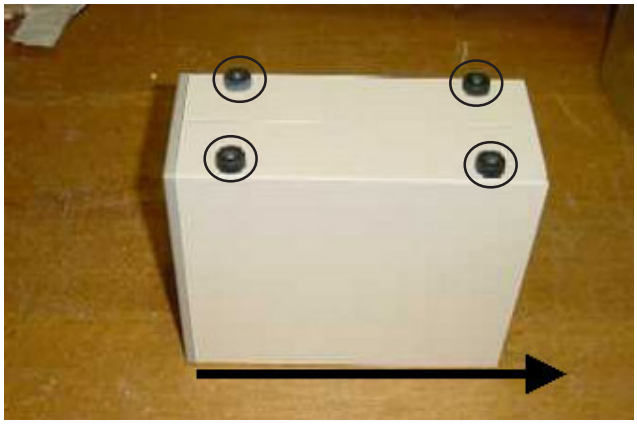

2. Hold the front panel and slide the enclosure backward. Remove the enclosure from the recorder unit. The inner block appears.

3. Open the paper magazine with the paper magazine release lever. There are 2 screws which secure the recorder sub assy to the recorder chassis through the bracket. Remove the 2 screws and remove the bracket from the recorder unit.

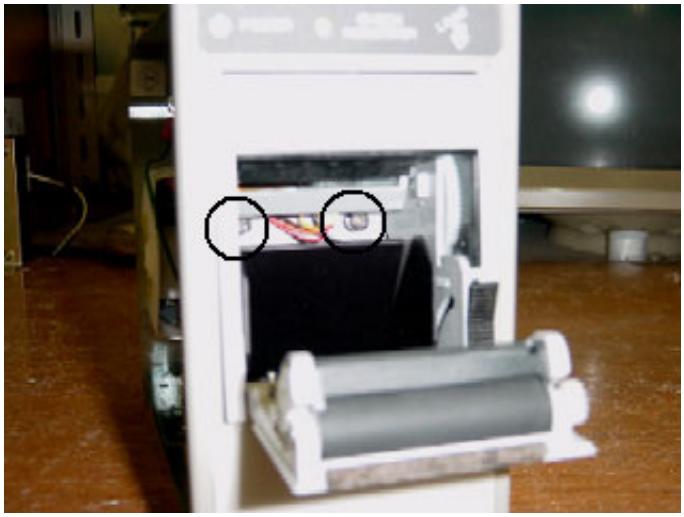

4. Pull the recorder sub assy toward you until you can see 2 screws at the bottom of the recorder sub assy.

5. Remove the 2 screws which secure the paper tray to the recorder sub assy and remove the paper tray from the recorder sub assy.
6. Disconnect the flat cable between the recorder sub assy and RS232C interface board. Remove the recorder sub assy from the recorder unit.

Removing the AC Inlet Socket

1. Remove the enclosure from the recorder unit according to the “Removing the Recorder Sub Assy” steps 1 to 2.
2. Remove the insulation cover from the AC inlet socket.
3. Insert a small flat-blade screwdrivers into the AC inlet socket upper clearance to release the upper latch of the AC inlet socket.
4. Insert a small flat-blade screwdrivers into the AC inlet socket lower clearance to release the lower latch of the AC inlet socket. Remove the AC inlet socket from the recorder unit.

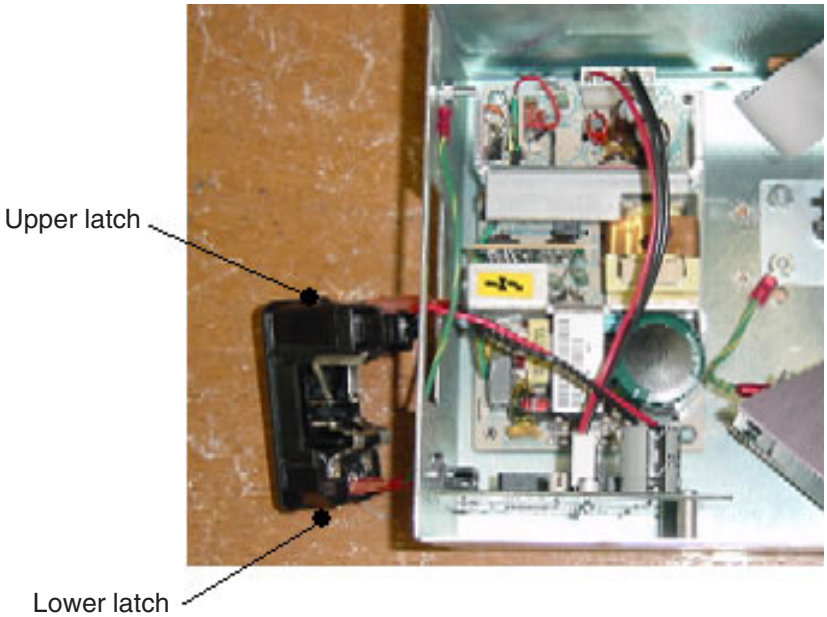

Removing the RS232C Interface Board

1. Remove the AC inlet socket from the recorder unit according to the “Removing the AC Inlet Socket”.
2. Remove the screw which secures the RS232C interface board to the recorder chassis.
3. Remove the board from the recorder unit.

Removing the Power Supply Unit

1. Remove the AC inlet socket from the recorder unit according to the “Removing the AC Inlet Socket”.
2. Remove the screw which secures the power supply unit to the recorder chassis.
3. Remove the power supply unit from the recorder unit.

Removing the Front Panel

1. Remove the recorder sub assy from the recorder unit according to the “Removing the Recorder Sub Assy”.
2. Remove the 2 screws which secure the front panel to the recorder chassis.
3. Remove the front panel from the recorder unit.

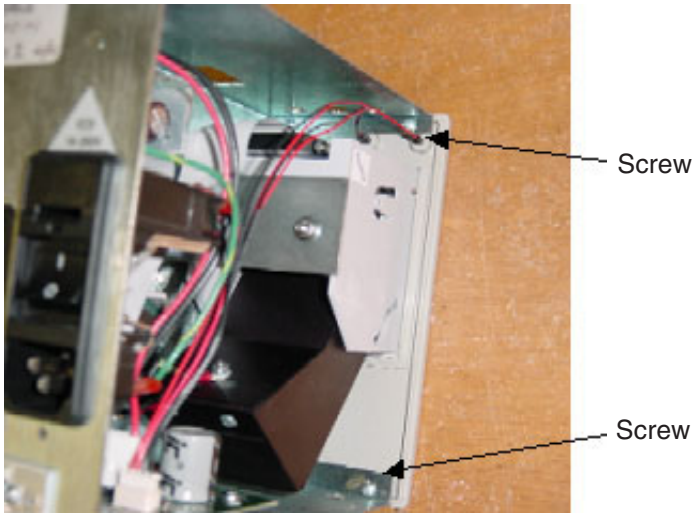

NOTE

When the front panel is replaced with a new one, the Nihon Kohden model number label also must be replaced with a new one.

Replacing the LED

1. Remove the enclosure from the recorder unit according to the “Removing the Recorder Sub Assy” steps 1 to 2.
2. Peel off the LED cover sheet on the upper part of the front panel.

3. Push the LED inward through the hole of the front panel and pull the LED rearward.

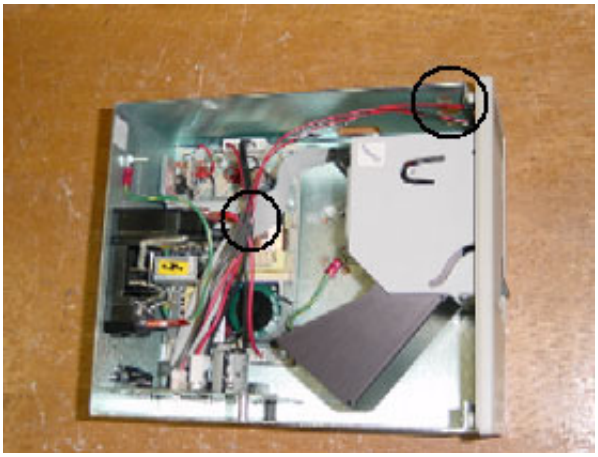

4. Cut the middle of the LED lead wire soldered to the RS232C interface board.
5. Replace the LED with a new one. Solder the LED lead wire to the remaining lead wire connected to the RS232C interface board. Cover the soldered point with insulated tape.
6. Assemble the recorder unit by reversing the above procedure, steps 3 to 1.

Replacing the Platen Roller/Bushings/Gear

1. Open the paper magazine with the paper magazine release lever. The paper guide and assembly of the roller, bushings and gear are in the recorder sub assy.
2. Pull both edges of the roller guide outward as shown below and remove the paper guide from the recorder sub assy.

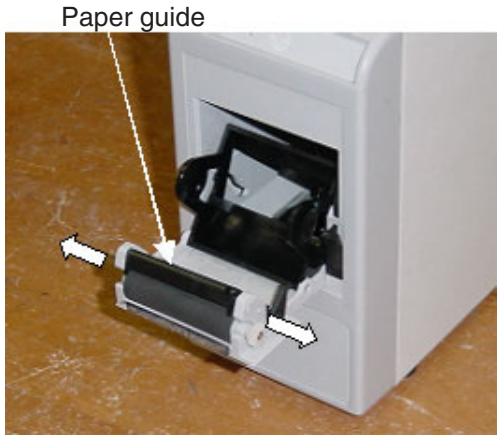

3. Insert a small flat-blade screwdriver into the space between the gear and frame of the paper magazine as shown below. Pry up the assembly of the roller, bushings and gear with the screwdriver until the assembly pops out.

4. Remove the roller, bushings and gear from the assembly. Replace the roller, bushings or gear with a new one and assemble the recorder unit by reversing the above procedure.

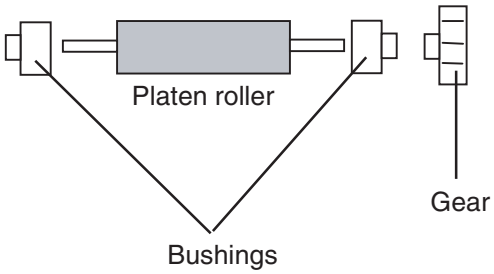

Cleaning the Thermal Array Head/Paper Sensor

1. Open the paper magazine with the paper magazine release lever. The thermal array head and paper empty sensor are in the recorder sub assy.

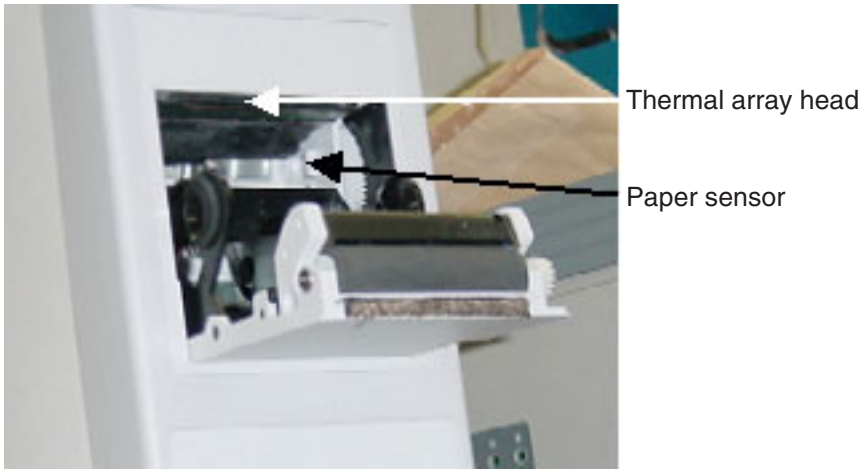

2. Clean the head and sensor with a cotton swab moistened with alcohol.

CAUTION

Since there is no adjustment which you can do, cleaning the thermal array head or paper sensor is the only thing you can do if the head or sensor has a problem.

Operation Check after Assembling the Recorder Unit

Check the recorder operation after assembling the recorder unit according to the following check list.

No.	Operation check	Check result
1	Check that the POWER lamp LED is lit when you turn on the recorder unit.	OK, NG
2	Check that the recording functions are available at the central monitor connected to the recorder unit.	OK, NG
3	Check that there is no paper skewing when the paper comes out.	OK, NG
4	Check that there is no uneven record density on the paper.	OK, NG
5	Check that the CHECK RECORDER lamp LED is lit when disconnecting the cable between the recorder unit and central monitor.	OK, NG

This page is intentionally left blank.

Section 5 Maintenance

To Be Replaced Periodically 5.1
Maintenance Check Items and Schedule 5.1
- External and Connection 5.2
- Display 5.2
- Sound 5.2
- Operation 5.3
- Data Storage 5.3
- Network Communication 5.4
- Recorder 5.4
- Laser Printer 5.4
- UPS 5.5
- Safety 5.5

This page is intentionally left blank.

To Be Replaced Periodically

We recommend the periodic replacement of the following components according to the expected life span.

NK Code No.	Description	Expected Life Span
677402*	Hard disk	Every 2 years (or 20,000 working hours if the working time is managed). If a defective sector is found on the hard disk within the one year, immediately replace it with a new hard disk.
636509**		
636545	Fan for chassis	Every 2 years (or 20,000 working hours if the working time is managed).

* Only for MU-971RA main unit of Vorax5001

** For others

Maintenance Check Items and Schedule

Perform this maintenance check once every six months.

A maintenance check sheet is provided at the end of this section. Make a copy of this check sheet before using it.
The check items are grouped as follows:

- External and Connection
- Display
- Sound
- Operation
- Data Storage
- Network Communication
- Recorder
- Laser Printer
- UPS
- Safety

External and Connection

Item	Check	Countermeasure against negative result
Dust on the fans	Check that there is no dust at the fan on the rear of the main unit and in the power supply unit.	If the fans get dusty, remove the dust not only from the fans but also from the inside of the main unit.
Crack or damage	Check that there is no crack and damage on each unit and peripheral accessories.	If there is a crack or damage, replace the cracked or damaged part with a new one.
Damaged switch or switch cover	Check that there is no physically damaged switch and switch cover.	If any switch or switch cover is damaged, replace it with a new one.
Protection key connection	Check that the protection key is firmly connected to the main unit through the connection cable.	If there is poor contact between the protection key and cable or between the cable and main unit, disconnect and firmly re-connect them.
Overall connection	Check that each connection of the main unit, mouse, keyboard, display unit and recorder unit is tight.	If the connection of the mouse or keyboard is loose or disconnected from the main unit, turn off the main unit according to the shut down procedure described in the operator's manual and firmly connect the mouse and keyboard to the main unit. Otherwise, there can be a damage on the main unit, mouse or keyboard by connecting them again while the power is turned on.
Power lamp	Check that the power lamp on the front panel is lit when turning on the main unit.	If the power lamp does not light, remove the cause.

Display

Item	Check	Countermeasure against negative result
Screen position	Check that the upper, lower, right and left edges of the screen meet the corresponding edges of the display area.	If the display position of the screen is not acceptable and the VL-971R display unit is used, perform the automatic adjustment. Refer to Section 6 "Adjustment".
First screen after power-on	Check that the All Bed screen appears when the main unit is turned on.	Remove the cause if the All Bed screen does not appear.

Sound

Item	Check	Countermeasure against negative result
QRS and alarm sounds	Check that the QRS sound and alarm sound volume can be adjusted on the System Setup screen.	If not, remove the cause.
Click sound	Check that a click sound is generated from the main unit when touching a key on the touch screen.	If not, remove the cause.

Operation

Item	Check	Countermeasure against negative result
Mouse	Check that the mouse operation is normal.	If not, remove the cause.
Keyboard	Check that the keyboard operation is normal.	If not, remove the cause.
Touch screen	Check that the touch screen operation is normal.	If not, remove the cause.
Calibration of the touch screen	Check that the touch screen can be calibrated. Refer to "Calibrating the Touch Screen" in Section 2 "Troubleshooting".	If the touch screen cannot be calibrated, remove the cause. Refer to "Touch Screen Problem" in Section 2 "Troubleshooting".
Dirt on the touch screen	Check that the touch screen has no dirt.	If the touch screen gets oily, wipe it with a soft cloth moistened with diluted neutral detergent.

Data Storage

Item	Check	Countermeasure against negative result
Trendgraph and tabular data	Check that the trendgraph and tabular data from each bedside monitor are displayed on the screen.	Remove the cause if not.
Arrhythmia recall and ST recall data	Check that the arrhythmia recall and ST recall data from each bedside monitor are displayed on the screen.	Remove the cause if not.
Data storage with the optional program	When the optional program kit is installed into the main unit, check that the additional function works. For example, when the full disclosure program or 12-lead ECG interpretation filing program is installed, check that the corresponding window is displayed on the screen by touching the corresponding key on the Menu screen. When the 12 or 16 patient expansion program is installed, check that the 12 or 16 Patients key is added in the "Display Setting" window on the System Setup screen and the added key functions to display the 12 or 16 patients on the All Bed screen.	Remove the cause if the additional function does not work.

Network Communication

Item	Check	Countermeasure against negative result
Communication between the central and bedside monitors	Check that the monitored beds* which are registered in the "Monitored Beds" window on the System Setup screen are displayed on the All Bed screen.	Remove the cause if one of the monitored beds is not displayed.

*The bedside monitors must be turned on.

Recorder

Item	Check	Countermeasure against negative result
Missing dots	Check that the waveform and numeric data recorded on the paper have no missing dots.	If they have missing dots, remove the cause. Refer to "Recorder Problem" in Section 2 "Troubleshooting".
Paper snaking	Check that the recording paper comes out without snaking.	If the paper snakes, remove the cause.
Power lamp	Check that the power lamp is lit when turning on the recorder.	If the lamp is not lit, remove the cause.
CHECK RECORDER lamp	Check that the CHECK RECORDER lamp lights when opening the paper magazine.	If the lamp does not light, remove the cause.

Laser Printer

Item	Check	Countermeasure against negative result
Print key function	Check that the trendgraph of a selected patient is printed with the print key at the bottom of the screen.	If the trendgraph is not printed, remove the cause.
Paper jam	Check that there is no paper jam at the laser printer.	If the laser printer has a paper jam, remove the cause.

UPS

Item	Check	Countermeasure against negative result
Connection to the UPS	Check that the power cords of the main unit, display unit and recorder unit are connected to the UPS. Refer to "Connection Diagram" in Section 1 "General".	Connect the main unit, display unit and recorder unit to the UPS with each power cord.
Disconnection from the UPS	Check that the laser printer is not connected to the UPS.	Do not connect the laser printer to the UPS.
Output voltage from the UPS	Check that the line voltage within the range of ±10% is output from the UPS when the UPS power cord is disconnected from the mains voltage.	If the output is out of the range, remove the cause. Refer to "Power Problem" in Section 2 "Troubleshooting".
Lifetime of the UPS battery	Check that the UPS battery is not expired.	If the battery life time described in the UPS operator's manual has expired, ask the user to accept the battery replacement or replace the battery with a new one.

Safety

Item	Check	Countermeasure against negative result
Protective earth terminal	Check that the protective earth terminal of the UPS is grounded.	Ground the protective earth terminal of the UPS.
Earth leakage current of the main unit (refer to IEC 60950)	Check that the earth leakage current does not exceed 3.5 mArms under normal condition.	Remove the cause if the earth leakage current exceeds the maximum value.
Earth leakage current of the VL-971R/RK display unit (refer to IEC 60601-1)	Check that the earth leakage current does not exceed 0.5 mArms under normal condition and 1.0 mArms under each single fault condition.	Remove the cause if the earth leakage current exceeds one of the maximum values.

Maintenance Check Sheet

(Refer to the Maintenance section of the service manual for details.)

Customer: _____ Customer Address: _____
Service Personnel: _____ Service Company: _____
Instrument Name: _____ Instrument Model: _____
Instrument Serial Number: _____ Hardware Revision: _____
Software Version: _____

External and Connection

There is no dust at the fan on the rear of the main unit and in the power supply unit.
There is no crack and damage on each unit and peripheral accessories.
There is no physically damaged switch or switch cover.
The protection key is firmly connected to the main unit through the connection cable.
Each connection of the main unit, mouse, keyboard, display unit and recorder unit is tight.
The power lamp on the front panel lights when turning on the main unit.

Display

The upper, lower, right and left edges of the screen meet the corresponding edges of the display area.
The All Bed screen appears when the main unit is turned on.

Sound

The QRS sound and alarm sound volume can be adjusted on the System Setup screen.
A click sound is generated from the main unit when touching a key on the touch screen.

Operation

The mouse and keyboard operation is normal.
The touch screen operation is normal.
The touch screen is calibrated.
The touch screen has no dirt.

Data Storage

The trendgraph and tabular data from each bedside monitor are displayed on the screen.
The arrhythmia recall and ST recall data from each bedside monitor are displayed on the screen.
The additional function works when the optional program kit is installed in the main unit.

Network Communication

The monitored beds* which are registered in the “Monitored Beds” window on the System Setup screen are displayed on the All Bed screen.

Recorder

The waveform and numeric data recorded on the paper have no missing dot.
The recording paper comes out without snaking.
The power lamp is lit when turning on the recorder.
The CHECK RECORDER lamp lights when opening the paper magazine.

Laser Printer

The trendgraph of a selected patient is printed with the print key at the bottom of the screen.
There is no paper jam at the laser printer.

UPS

The power cords of the main unit, display unit and recorder unit are connected to the UPS

The laser printer is not connected to the UPS.

The line voltage within the range of ±10% is output from the UPS when the UPS power cord is disconnected from the mains voltage.

The UPS battery is not expired.

Safety

The protective earth terminal of the UPS is grounded.

Earth leakage current of the main unit is less than prescribed limits.

Earth leakage current of the display unit is less than prescribed limits.

This page is intentionally left blank.

Section 6 Adjustment

Adjusting the VL-971R Display Unit 6.1
Automatic Adjustment 6.1
Manual Adjustment 6.2

This page is intentionally left blank.

Adjusting the VL-971R Display Unit

When a CRT display unit is used with a personal computer, adjustment of the CRT display unit is not required. However, when an LCD display unit is used with a personal computer, adjustment at the LCD display unit is usually required for clear screen display.

Newer LCD display units have automatic screen adjustment which handles the RGB output signals from most personal computers within an acceptable range. To more clearly display the screen, the LCD display units also have manual screen adjustment. The VL-971R display unit has both automatic and manual screen adjustments.

This display unit accepts the analog RGB signals. The red, green and blue primary color signals are individually input to the display unit. The combination of primary colors makes the different colors as shown below.

Code	Display Color	Combination of Primary Color(s)
1	Blue	Blue
2	Red	Red
3	Purple	Blue and red
4	Green	Green
5	Light blue	Blue and green
6	Yellow	Red and green
7	White	Blue, red and green

According to the above table, you can judge which primary color has something wrong when a color problem occurs.
For example, if the display color which should be white is yellow, the blue color signal has a problem. However, to specify which part, i.e. display unit, main unit or cable between them, has a problem, you have to replace the unit or cable with a known good compatible unit or cable one at a time.

Automatic Adjustment

When the screen display is not normal, do the following procedure so that the screen display settings are automatically adjusted. Refer to “LCD Unit VL-971R/RK” of the “Panel Descriptions” in Section 1.

1. Check that the RGB signals are input to the display unit.
2. Press the S (Video Source) button on the rear of the display unit. The adjustment window appears on the screen.
3. Check that “Computer” is selected in the window and highlighted in yellow.
4. Press the Down/Left button twice. The screen display settings such as the horizontal and vertical synchronization settings are automatically adjusted. If the RGB signals are poor or the RGB output signals from the main unit are not appropriate for the display unit, manual adjustment is also required.

Manual Adjustment

After performing the automatic adjustment, perform the following procedure.

1. Check that the CNS system program is running.
2. Select “Horizontal Position” from the setting items.
3. Adjust the horizontal position so that the left edge of the screen meets the left edge of the LCD display area.
4. Use a magnifying glass and check that there is no position difference between the left edges.
5. Select “Horizontal Size” from the setting items.
6. Adjust the horizontal size so that the right edge of the screen meets the right edge of the LCD display area.
7. Use a magnifying glass and check that there is no position difference between the right edges.
8. Select “Focus” from the setting items.
9. Adjust the focus so that the entire screen is most clearly displayed. If the focus setting is not optimal, the screen blurs.
10. Select “Color Temperature Menu” from the setting items and select each primary color in the color temperature menu to adjust the color tone.

NOTE

When the primary color has something wrong, usually it is caused by a failure of the display unit, main unit or cable between them. Solving the problem with the color tone adjustment is rare.

Section 7 Replaceable Parts List

MU-971RA/RJ/RK Main Unit (Vorax5000) 7.2
MU-971RA/RJ/RK Main Unit (Vorax5001) 7.4
VL-971R/RK Optional Display Unit 7.6
WS-971R Optional Recorder Unit 7.8

This page is intentionally left blank.

When ordering parts or accessories from your nearest Nihon Kohden Corporation distributor, please quote the NK code number and part name which are listed in this service manual, and the name or model of the unit in which the required part is located. This will help us to promptly attend to your needs. Always use Nihon Kohden parts and accessories to assure maximum performance from your instrument.

MU-971RA/RJ/RK Main Unit (Vorax5000)

Index	NK Parts Code	Description
1	635689	Power supply unit PCSA-300P-X2S
2	635698*	Motherboard MX3SP A-OPEN
	372321A	Lithium battery CR-2032
3	633094	1 GHz CPU Pentium3 with fan and heat sink
4	636492	256 MB DIMM SDRAM
5	636483	3.5" 1.4 MB floppy disk drive
6	636509	40 GB IDE hard disk
7	636518	CD-ROM drive
8	636527**	Graphic board RADEON 32 ATI
	644429	Fan for graphic board
9	638926	Serial interface board CYBER SERIAL
10	636536	PC chassis IW-V500
11	636545	Fan for chassis
12	660714	Fan for CPU Pentium3

* Lithium battery is included but CPU with fan and heat sink (Index No. 3) and SDRAM (Index No. 4) are not included.

** Fan for graphic board is included.

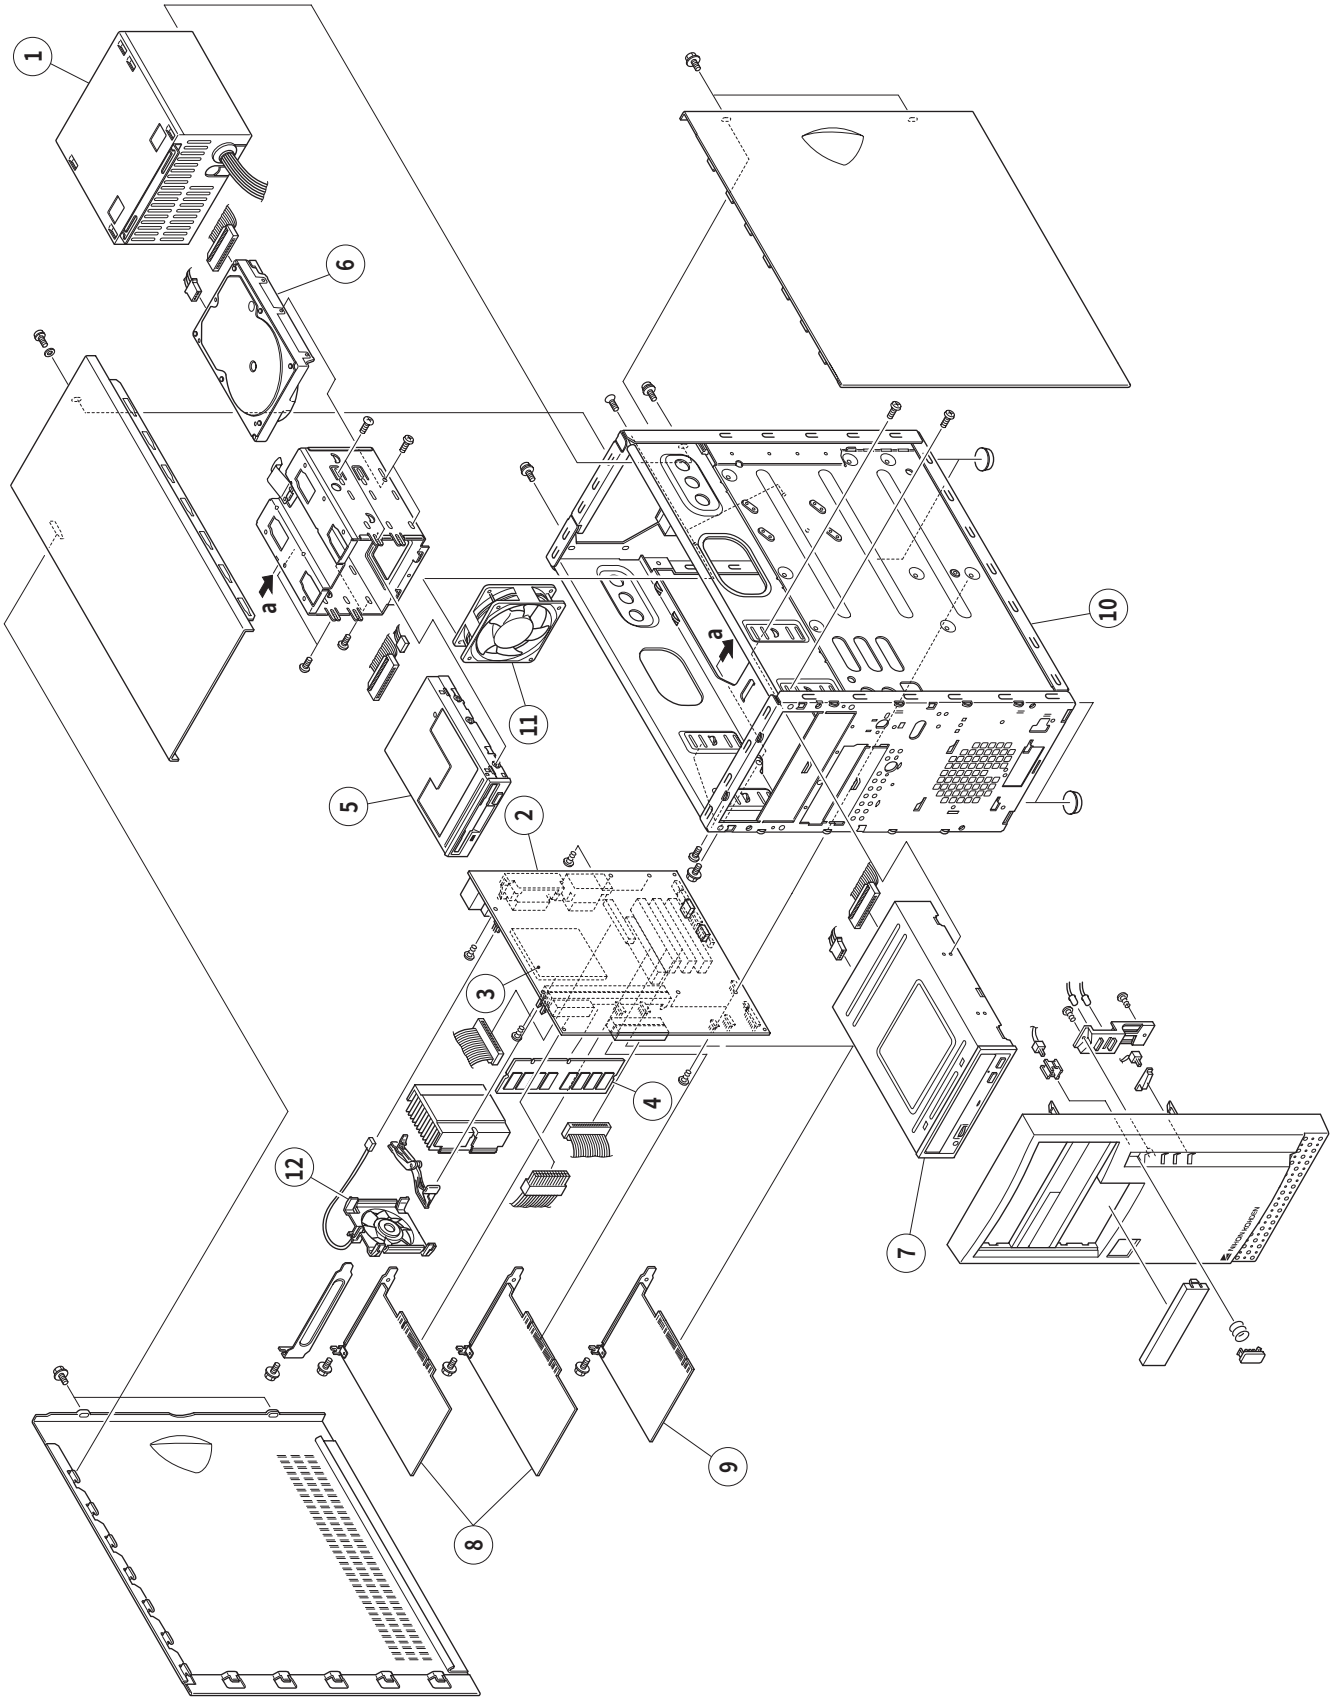
1
6
a
a
10
11
5
2
3
4
12
7
9
8

MU-971RA/RJ/RK Main Unit (Vorax5001)

Index	NK Parts Code	Description
1	658691	Power supply unit PCSA-300P-X2V
2	658708*	Motherboard MX4BR-533 A-OPEN
	372321A	Lithium battery CR-2032
3	658717A	2.4 GHz CPU Pentium IV with fan and heat sink
4	658726	256 MB DDR266 SDRAM
5	636483	3.5" 1.4 MB floppy disk drive
6	677402**	250 GB IDE hard disk
	636509***	40 GB IDE hard disk
7	636518	CD-ROM drive
8	658735	Graphic board RADEON 7000 PCI
9	638926	Serial interface board CYBER SERIAL
10	658744	PC chassis IW-V500G
11	636545	Fan for chassis
12	669189	Fan for CPU Pentium IV

* Lithium battery is included but CPU with fan and heatsink (Index No. 3) and SDRAM (Index No. 4) are not included.

** Only for MU-970RA main unit of Vorax5001

*** For others

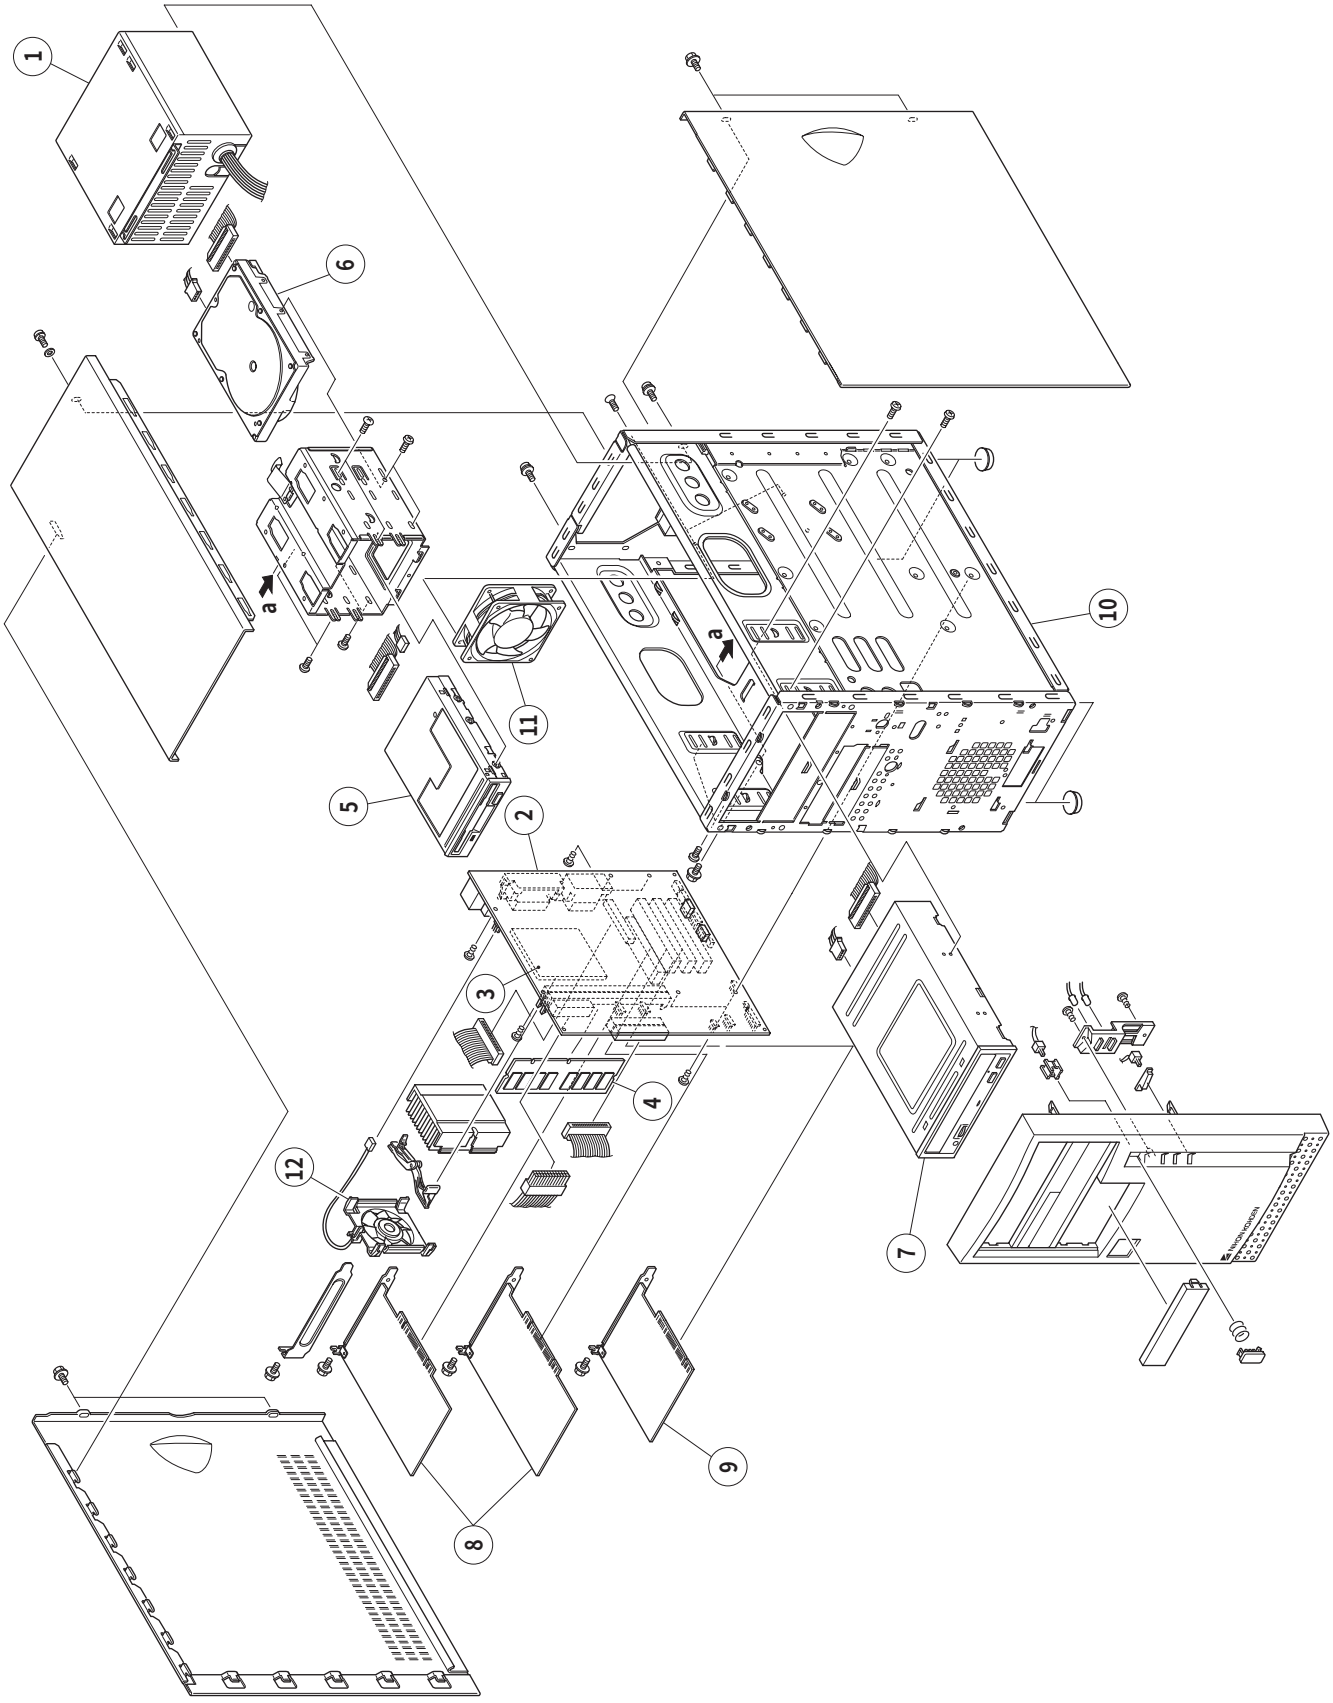
1
6
a
a
10
11
5
2
3
4
12
7
9
8

VL-971R/RK Optional Display Unit

Index	NK Code No.	Qty	Description
1	646124	1	LCD assembly (backlight lamp included)
2	646133	1	Touch screen
3	646142	1	LCD control board
4	646151	1	Audio board
5	646178	1	Front cover
6	646187	1	Rear cover
7	646196	2	Joint cap
8	646204	4	Plastic bracket
9	646213	2	Speaker
10	646231	1	Digital RGB cable
11	646294	1	Connection cable between the LCD control board and key switch assembly
12	646222A	1	AC adapter
13	646249	1	Internal power supply cable
15	625477	1	Touch screen control board
16	625361	1	Power supply cable for touch screen control board
17	625432	1	Serial data cable
18	625379	1	Analog RGB cable
19	631826	1	Power switch
20	631817	1	Key switch assembly

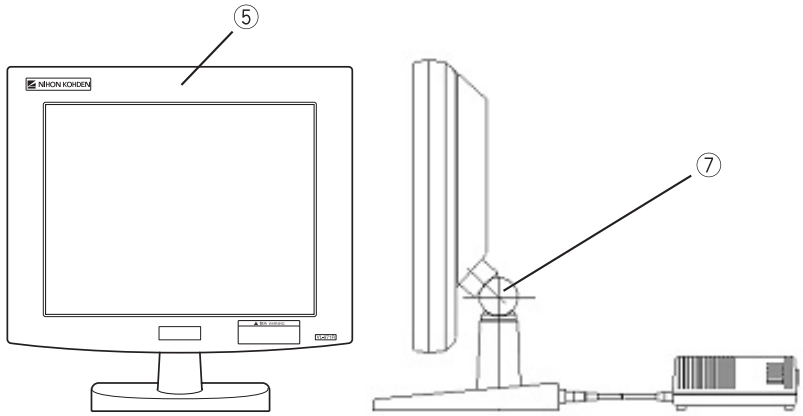
⑤
⑦

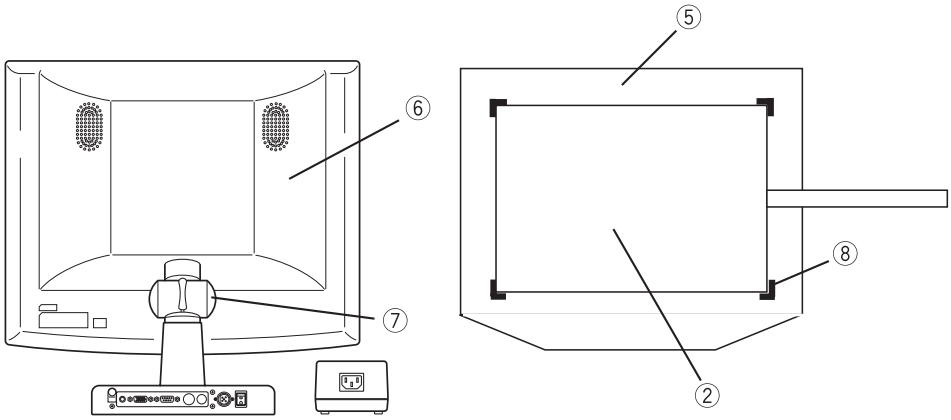
⑤
⑥
⑦
⑧
②

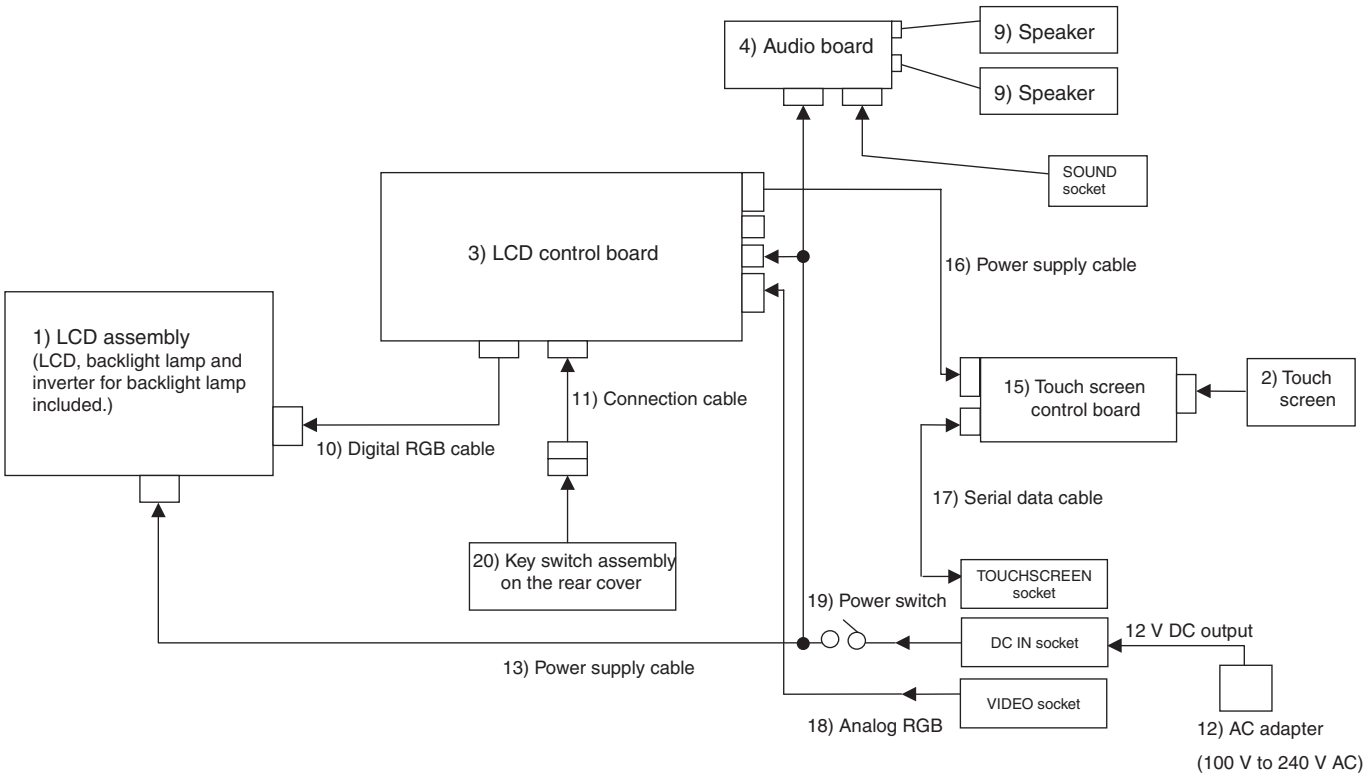
4) Audio board
9) Speaker
9) Speaker
SOUND socket
3) LCD control board
16) Power supply cable
1) LCD assembly
(LCD, backlight lamp and inverter for backlight lamp included.)
11) Connection cable
15) Touch screen control board
2) Touch screen
10) Digital RGB cable
17) Serial data cable
20) Key switch assembly on the rear cover
TOUCHSCREEN socket
19) Power switch
DC IN socket
12 V DC output
13) Power supply cable
VIDEO socket
18) Analog RGB
12) AC adapter
(100 V to 240 V AC)

WS-971R Optional Recorder Unit

Index	NK Code No.	Qty	Description
1	648808	1	Power supply unit
2	648817	1	RS232C interface board
3	648826	1	AC inlet socket with power switch
4	648835	1	Fuse cap
5	597177	2	Fuse
6	648853	1	Power supply cable for RS232C interface board
7	648862	1	AC line voltage supply cable between the AC inlet socket and power supply unit
8	648871	1	Connection cable between the RS232C interface board and recorder sub assy
9	648889	1	Green LED with lead wires
10	648898	1	Yellow LED with lead wires
11	648906	1	Connection cord for LEDs
12	648915	4	Rubber foot
13	648924	1	Enclosure
14	648933	1	Front panel
15	648942	1	Recorder sub assy
16	648951	1	Platen roller
17	648969	1	Gear
18	648978	2	Bushings
19	6124-036836	1	Model number label

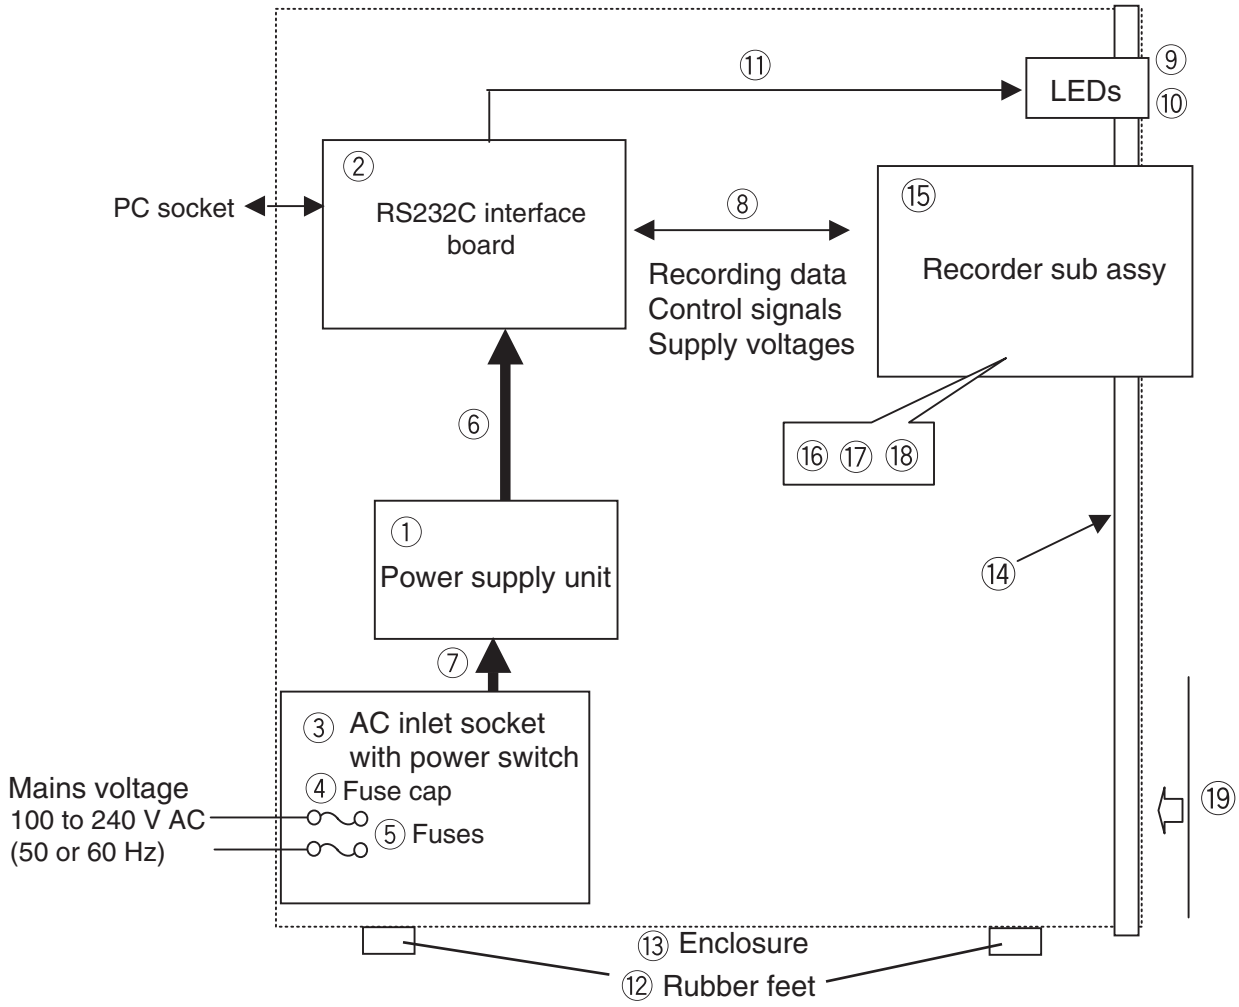
⑪
⑨
LEDs
⑩
②
PC socket
RS232C interface board
⑧
⑮
Recorder sub assy
Recording data
Control signals
Supply voltages
⑥
⑯ ⑰ ⑱
①
Power supply unit
⑭
⑦
③ AC inlet socket with power switch
④ Fuse cap
⑤ Fuses
Mains voltage
100 to 240 V AC
(50 or 60 Hz)
⑲
⑬ Enclosure
⑫ Rubber feet

This page is intentionally left blank.

Section 8 Network Settings

Network Setting Flowchart 8.2
Setting the IP Address on Each Instrument 8.3
    Manually Setting the IP Address of the Central Monitor 8.3
Installing the Laser Printer (Network Printer) 8.6
Connecting the Network System 8.12
Start the System 8.12
Checking the Network Connection on the Central Monitor 8.13
Assigning the Group Name and Bed Name 8.14
    Assigning a Bed Name/CNS Name 8.15
        Assigning a CNS Name to a Central Monitor 8.15
    Registering Group Names in the Central Monitor 8.15
    Assigning a Group Name 8.16
    Checking the Bed Name and Group Name Setting 8.16
Selecting the Monitored Beds 8.17
Changing Settings of System Setup, Patient Setting and Setup 8.19
Adding an Instrument to the Network During System Operation 8.20

This page is intentionally left blank.

This section describes how to set the following settings.

- IP address
- Install the laser printer (network printer) on the central monitor
- Check the network connection
- Assign a bed name and group name to the monitors.
- Select the monitored beds on the central monitor.
- Adding an instrument to the network during system operation

Network Setting Flowchart

1. Set the IP address on each instrument.
2. Connect the network system.
3. Start the system.
4. Install the laser printer (network printer) on the central monitor.
5. Check the network connection on the central monitor.
6. Assign the bed name or CNS name to each instrument.
7. Assign the group name to each instrument.
8. Select the monitored beds on the central monitor.
9. Set necessary settings on the central monitor.
10. Start system operation.

Setting the IP Address on Each Instrument

Each instrument in the network has an IP address for data communication. Duplicate IP addresses must not be present in the same network.

A unique IP address is assigned to each instrument at shipment. Therefore, there should be no duplicate IP addresses and usually the IP address does not need to be changed.

If the IP address needs to be changed due to the network management in the facility, the IP address can be changed manually.

CAUTION

The network must be managed by the network administrator. Make sure that each monitor in the network has a different IP address. Otherwise, data communication cannot be performed properly and it causes incorrect monitoring. When adding a monitor to an already operating network, the IP address of the monitor must be set before connecting the monitor to the network.

NOTE

- **To avoid communication trouble, do not connect the network cable to each instrument before IP address setting is complete.**
- **Contact your Nihon Kohden distributor or representative when changing the IP address manually.**

Manually Setting the IP Address of the Central Monitor

When IP addresses are managed by the network administrator in your hospital, they need to be changed manually. IP address is set in Windows 2000. You need to shut down the central monitor system before setting the IP address.

1. Shut down the central monitor system.

2. Click the “Network and Dial-up Connections” icon. Or, select Start → Settings → Control Panel → Network and Dial-up Connection. The “Network and Dial-up Connection” dialog box opens.

3. Click “Local Area Connection”. The “Local Area Connection Status” dialog box opens and shows the network connection status.

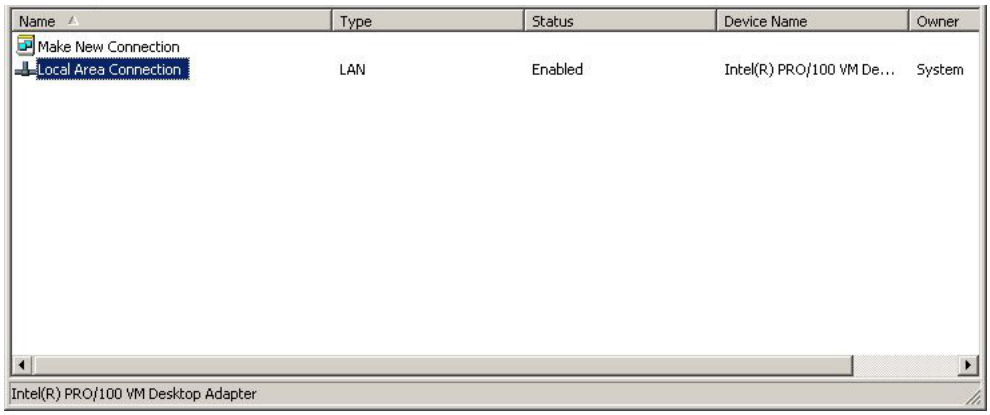

4. Click the “Properties” button. The “Local Area Connection Property” dialog box opens.

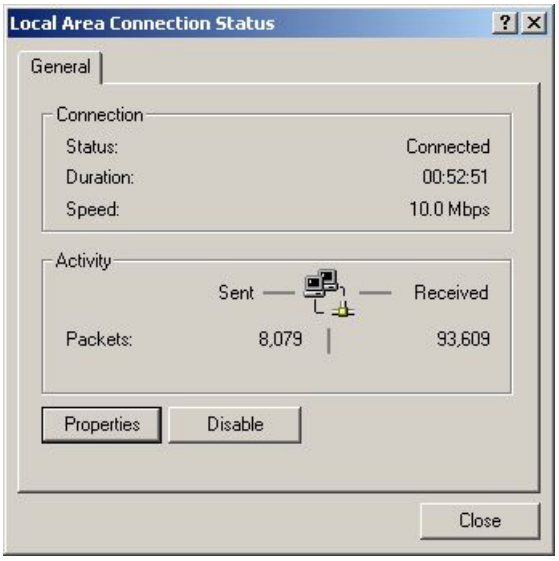

5. Click “Internet Protocol (TCP/IP)” to make it selected and click the “Properties” button. The “Internet Protocol (TCP/IP)” dialog box opens.

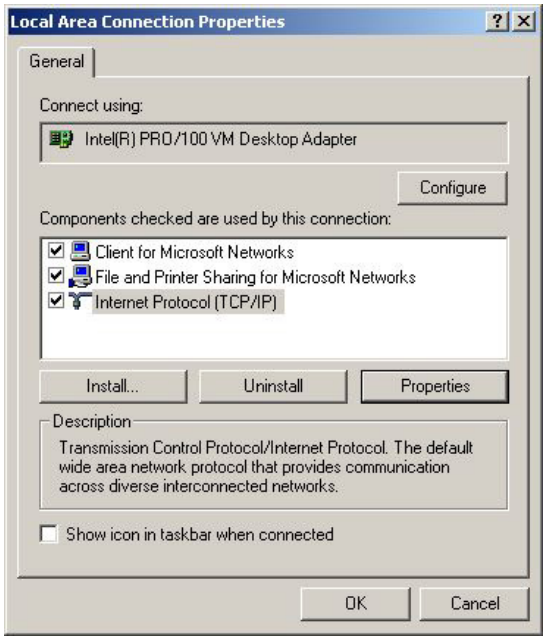

6. Enter the IP address and subnet mask.

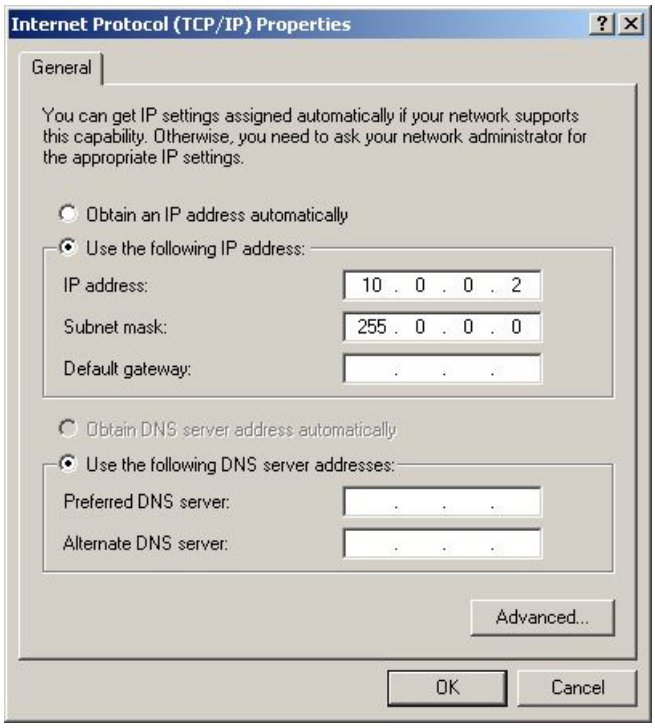
Internet Protocol (TCP/IP) Properties
General
You can get IP settings assigned automatically if your network supports this capability. Otherwise, you need to ask your network administrator for the appropriate IP settings.
Obtain an IP address automatically
Use the following IP address:
IP address:
10 . 0 . 0 . 2
Subnet mask:
255 . 0 . 0 . 0
Default gateway:
Obtain DNS server address automatically
Use the following DNS server addresses:
Preferred DNS server:
Alternate DNS server:
Advanced...
OK
Cancel

7. Click the “OK” button to finish setting.

8. Restart Windows 2000.

Installing the Laser Printer (Network Printer)

NOTE

The procedure in this section describes how to install a Hewlett Packard LaserJet 4000 series printer. When using other printers, refer to the printer manual.

Install the laser printer (network printer) in the central monitor. Shut down the central monitor system and set printer settings in Windows 2000.

NOTE

When more than one central monitor uses the printer, set the following settings on each central monitor. Connect the printer to each central monitor as a local printer, not as a network printer.

1. Shut down the central monitor system. Refer to Section 5 "Turning the Power Off".

2. Select Start → Settings → Printers. The "Printers" dialog box opens.

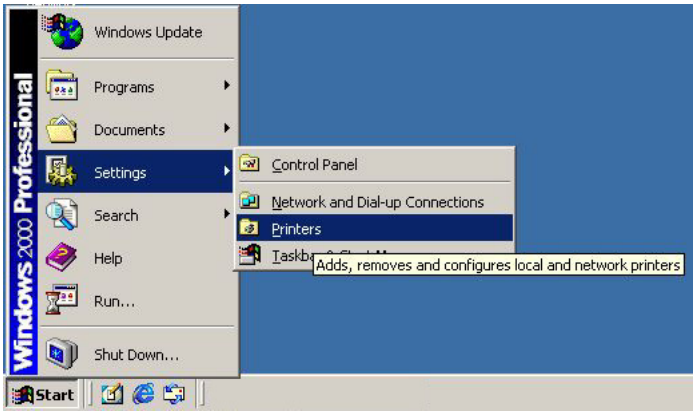

3. Click "Add Printer".

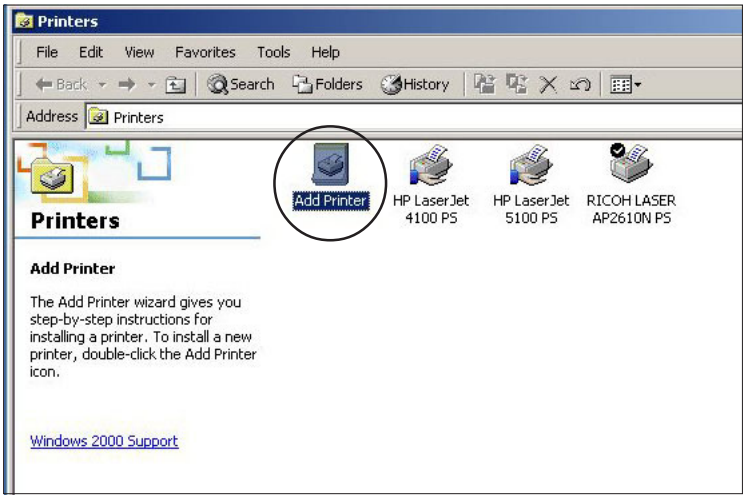
Printers
File Edit View Favorites Tools Help
Back Search Folders History
Address Printers
Add Printer
HP LaserJet 4100 PS
HP LaserJet 5100 PS
RICOH LASER AP2610N PS
Printers
Add Printer
The Add Printer wizard gives you step-by-step instructions for installing a printer. To install a new printer, double-click the Add Printer icon.
Windows 2000 Support

4. Click “Next” to start the “Add Printer Wizard”.

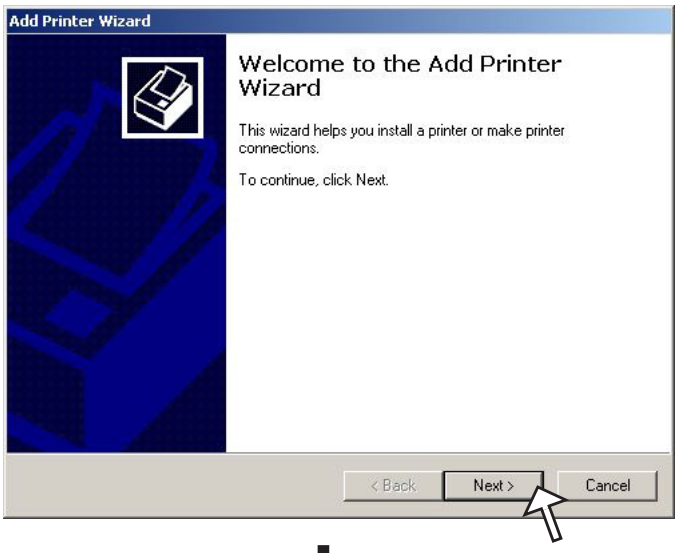
Add Printer Wizard
Welcome to the Add Printer Wizard
This wizard helps you install a printer or make printer connections.
To continue, click Next.
< Back
Next >
Cancel

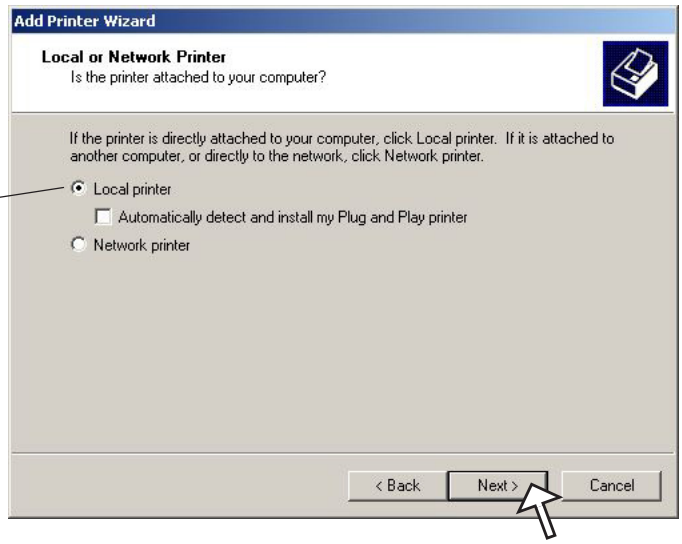
Add Printer Wizard
Local or Network Printer
Is the printer attached to your computer?
If the printer is directly attached to your computer, click Local printer. If it is attached to another computer, or directly to the network, click Network printer.
Local printer
Automatically detect and install my Plug and Play printer
Network printer
< Back
Next >
Cancel

Select “Local printer”.

5. Select “Use the following port”. Select the printer you use. (The IP address of the printer is in the Port column.) Click Next>.

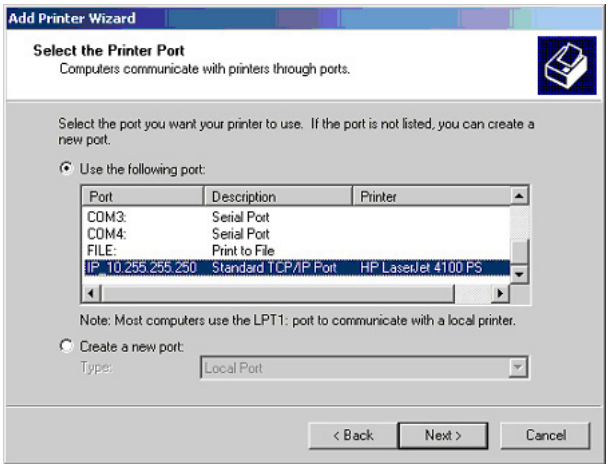

6. From Manufacturers, select HP. From Printers, select HP LaserJet 4000 Series PCL. (HP Laser Jet 4100n and HP Laser Jet 4200n use the same driver.) Click Next>.

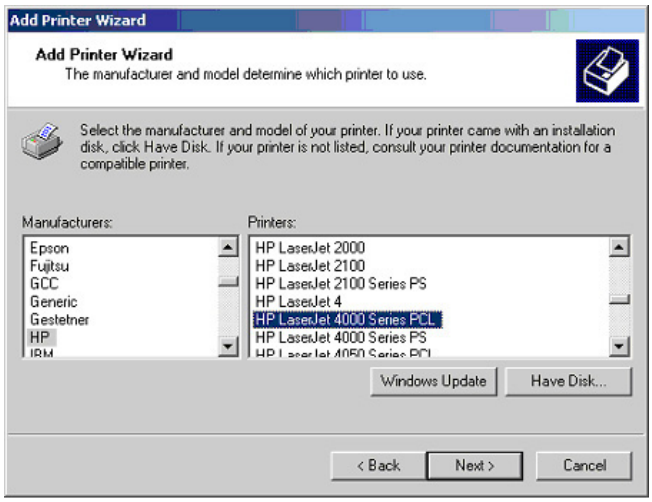
Add Printer Wizard
Add Printer Wizard
The manufacturer and model determine which printer to use.
Select the manufacturer and model of your printer. If your printer came with an installation disk, click Have Disk. If your printer is not listed, consult your printer documentation for a compatible printer.
Manufacturers:
Epson
Fujitsu
GCC
Generic
Gestetner
HP
Printers:
HP LaserJet 2000
HP LaserJet 2100
HP LaserJet 2100 Series PS
HP LaserJet 4
HP LaserJet 4000 Series PCL
HP LaserJet 4000 Series PS
Windows Update
Have Disk...
< Back
Next >
Cancel

7. Select “Replace existing driver” and click Next>.

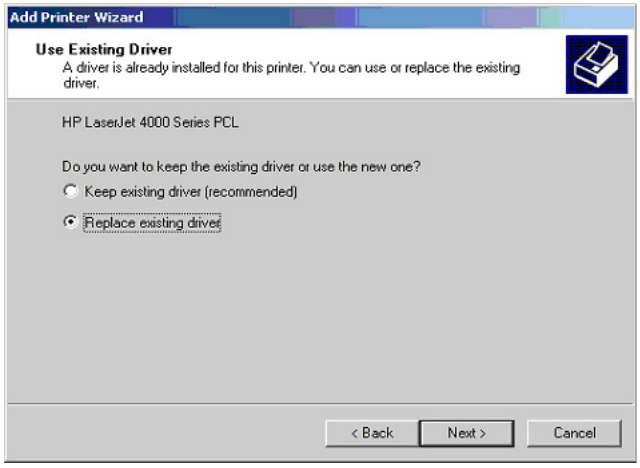
Add Printer Wizard
Use Existing Driver
A driver is already installed for this printer. You can use or replace the existing driver.
HP LaserJet 4000 Series PCL
Do you want to keep the existing driver or use the new one?
Keep existing driver (recommended)
Replace existing driver
< Back
Next >
Cancel

8. Select “Yes” and click Next>.

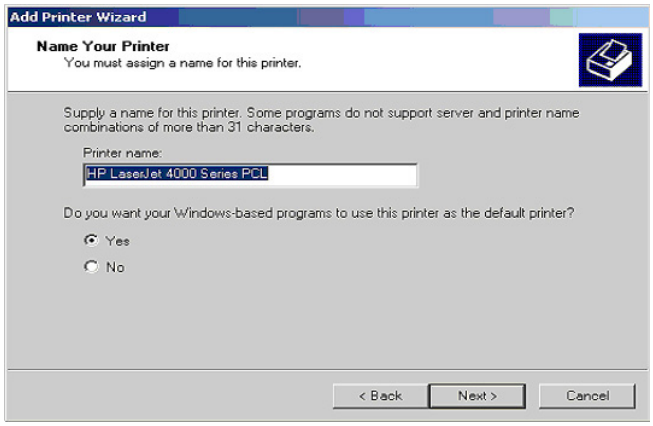
Add Printer Wizard
Name Your Printer
You must assign a name for this printer.
Supply a name for this printer. Some programs do not support server and printer name combinations of more than 31 characters.
Printer name:
HP LaserJet 4000 Series PCL
Do you want your Windows-based programs to use this printer as the default printer?
Yes
No
< Back
Next >
Cancel

9. Select “Do not share this printer” a

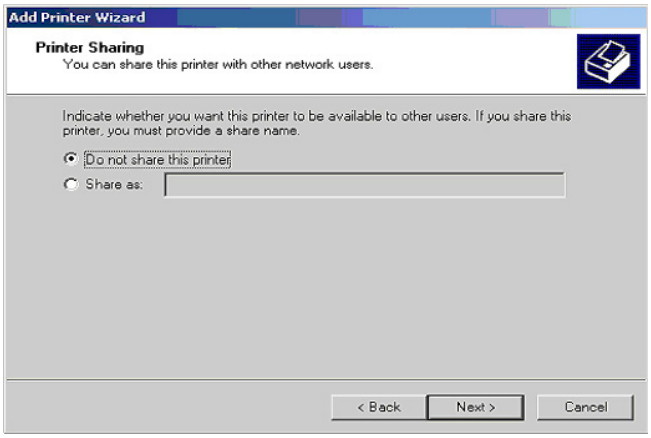
Add Printer Wizard
Printer Sharing
You can share this printer with other network users.
Indicate whether you want this printer to be available to other users. If you share this printer, you must provide a share name.
Do not share this printer
Share as:
< Back
Next >
Cancel

10. Select “Yes” and click Next>.

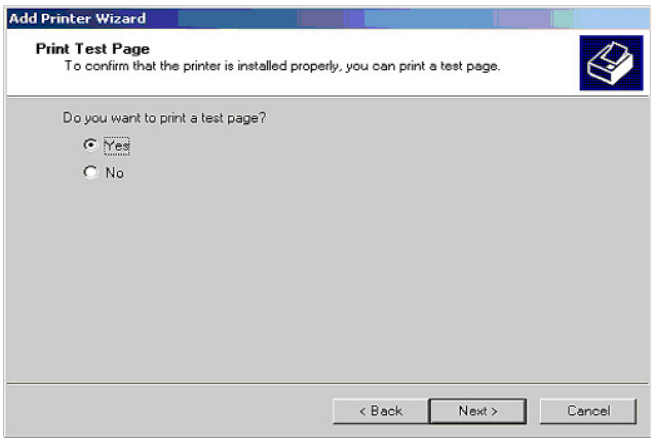
Add Printer Wizard
Print Test Page
To confirm that the printer is installed properly, you can print a test page.
Do you want to print a test page?
Yes
No
< Back
Next >
Cancel

11. Click Finish.

12. Files are copied and a test page is printed. After the test page is printed, click OK.

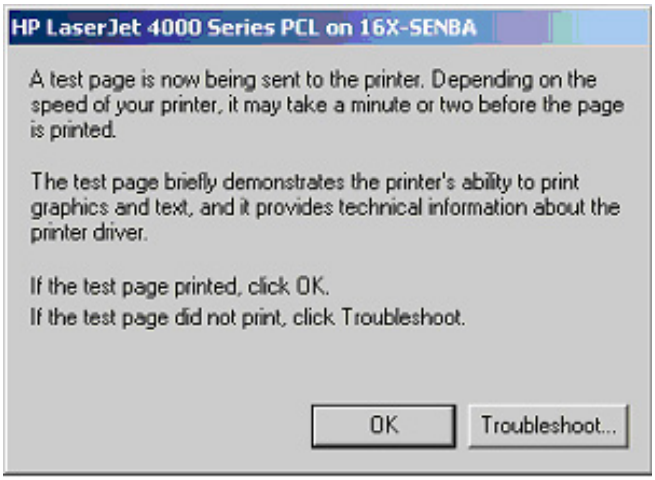
HP LaserJet 4000 Series PCL on 16X-SENBA
A test page is now being sent to the printer. Depending on the speed of your printer, it may take a minute or two before the page is printed.
The test page briefly demonstrates the printer's ability to print graphics and text, and it provides technical information about the printer driver.
If the test page printed, click OK.
If the test page did not print, click Troubleshoot.
OK
Troubleshoot...

13. On the Printers window, confirm that HP Laser Jet 4000 Series PCL is added with a check mark. Close the Printers window.

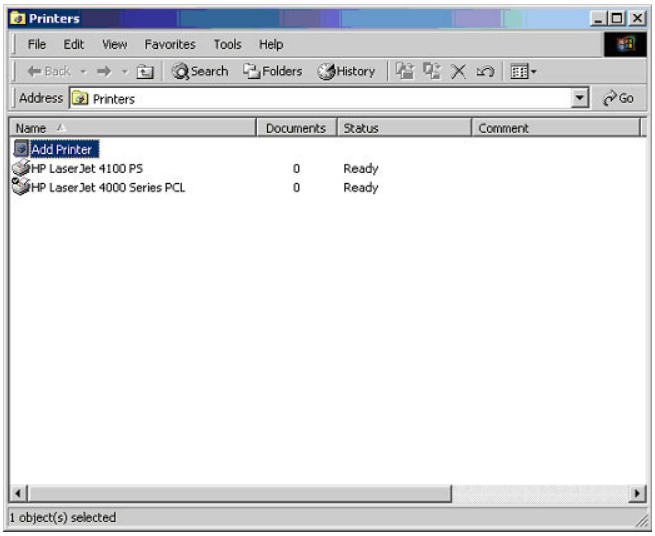

14. Shut down the window and restart it. Select restart and click OK.

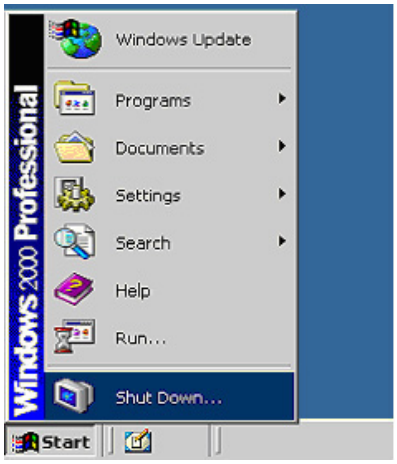

15. After the CNS-9701 system starts, print something to check the printer works.

Connecting the Network System

Refer to the Network and System installation guide and Section 3 “Connecting the Central Monitor to the Network System”.

Start the System

NOTE

Confirm that the “LINK” LED is lit on the hub and network connectors for each instrument. If it is not lit when each instrument is turned on, electrical connection is not complete. Confirm the wiring.

Turn on the power of the instruments in the following order.

1. UPS

2. These instruments can be turned on in any order.
   - Central monitor main unit
   - LCD unit
   - Recorder unit

The following instruments can be turned on at any time.
- Laser printer
- Multiple patient receiver
- Bedside monitors and transmitters

Checking the Network Connection on the Central Monitor

You can see the network connection on the Maintenance window of the System Setup on the central monitor. All instruments which are connected to the network and are turned on are listed on the Maintenance window of the System setup. Confirm the number of connected instruments.

1. Touch “System Setup” to display the System Setup screen.

2. Enter the password.

The password is displayed as ****.

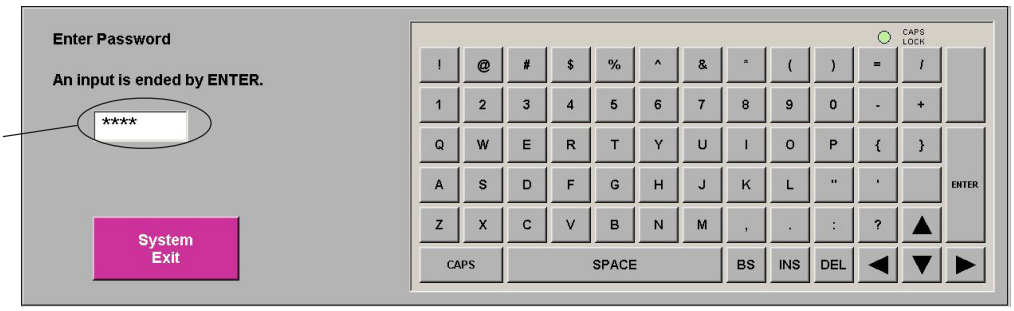

3. Touch “Maintenance”. The Maintenance window opens and network information is displayed.

Instrument’s name (bed name or CNS name)

IP address

Group name

Touch to reload the latest information

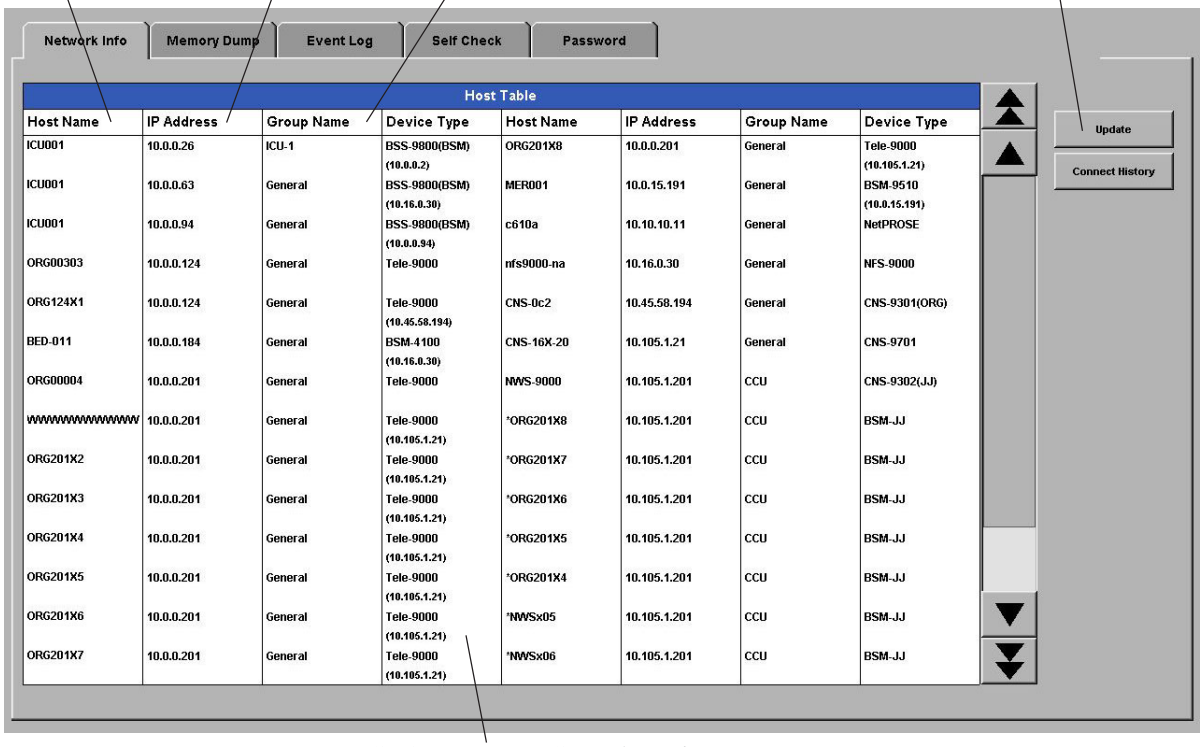

Host Name	IP Address	Group Name	Device Type	Host Name	IP Address	Group Name	Device Type
ICU001	10.0.0.26	ICU-1	BSS-9800(BSM) (10.0.0.2)	ORG201X8	10.0.0.201	General	Tele-9000 (10.105.1.21)
ICU001	10.0.0.63	General	BSS-9800(BSM) (10.16.0.30)	MER001	10.0.15.191	General	BSM-9510 (10.0.15.191)
ICU001	10.0.0.94	General	BSS-9800(BSM) (10.0.0.94)	c610a	10.10.10.11	General	NetPROSE
ORG00303	10.0.0.124	General	Tele-9000	nfs9000-na	10.16.0.30	General	NFS-9000
ORG124X1	10.0.0.124	General	Tele-9000 (10.45.58.194)	CNS-0c2	10.45.58.194	General	CNS-9301(ORG)
BED-011	10.0.0.184	General	BSM-4100 (10.16.0.30)	CNS-16X-20	10.105.1.21	General	CNS-9701
ORG00004	10.0.0.201	General	Tele-9000	NWS-9000	10.105.1.201	CCU	CNS-9302(JJ)
WWWWWWWWWW	10.0.0.201	General	Tele-9000 (10.105.1.21)	*ORG201X8	10.105.1.201	CCU	BSM-JJ
ORG201X2	10.0.0.201	General	Tele-9000 (10.105.1.21)	*ORG201X7	10.105.1.201	CCU	BSM-JJ
ORG201X3	10.0.0.201	General	Tele-9000 (10.105.1.21)	*ORG201X6	10.105.1.201	CCU	BSM-JJ
ORG201X4	10.0.0.201	General	Tele-9000 (10.105.1.21)	*ORG201X5	10.105.1.201	CCU	BSM-JJ
ORG201X5	10.0.0.201	General	Tele-9000 (10.105.1.21)	*ORG201X4	10.105.1.201	CCU	BSM-JJ
ORG201X6	10.0.0.201	General	Tele-9000 (10.105.1.21)	*NWSx05	10.105.1.201	CCU	BSM-JJ
ORG201X7	10.0.0.201	General	Tele-9000 (10.105.1.21)	*NWSx06	10.105.1.201	CCU	BSM-JJ

Manual setting of a central monitor’s IP address is done on Windows 2000.

CNS-XXXX: Central monitor (system)
BSM-XXXX: Bedside monitor
Tele-9000: beds whose data is received via the ORG-9200 multiple patient receiver or transmitter.
(An IP address in parenthesis is the address where the bed’s data is saved.)

Assigning the Group Name and Bed Name

To identify the monitors, each monitor has an instrument name (bed name/CNS name) and a group name. Every bed and every central monitor belongs to one of up to 16 groups. A local bed is assigned to the same group as the central monitor.

Groups are provided to simplify bed selection in large hospitals. It is recommended to assign a different bed name to each bed and central monitor so that it is easy to identify a bed.

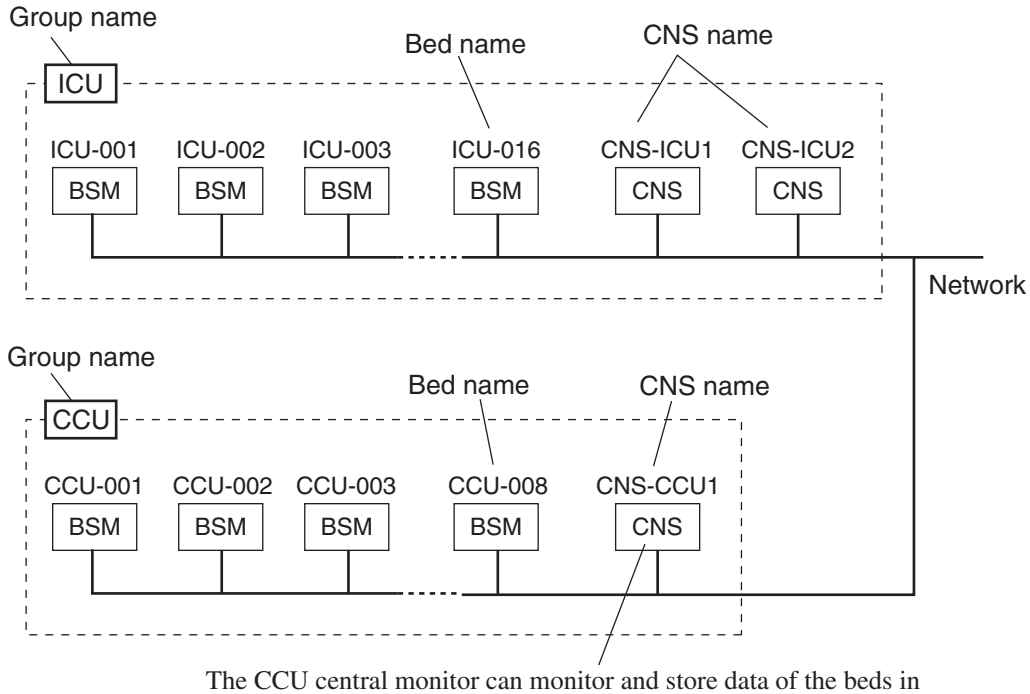

The CCU central monitor can monitor and store data of the beds in the ICU group. However, it is recommended to monitor and store data of the CCU beds in the CCU group so that data will not be lost.

CAUTION

When the monitor is connected to a central network, set the bed name/ CNS name and group name on the monitor to correctly identify the bed on the central monitor. Otherwise the monitor cannot be managed properly.

Assigning a Bed Name/ CNS Name

Assign an instrument name to the central monitor, beds on the multiple patient receiver and bedside monitors on the network.

Central monitor:
Exit the central monitor system and assign a name in Windows 2000.

Beds on the ORG-9200 multiple patient receiver:
First register the bed as a monitored bed on the Monitor Setting window of the System Setup. Then set the name for the bed. For the procedure, refer to the CNS-9701 operator's manual.

Bedside monitors:
Assign the bed name to bedside monitors on the SYSTEM SETUP screen on each bedside monitor. Refer to the bedside monitor operator's manual.

Assigning a CNS Name to a Central Monitor

1. Shut down the central monitor system.
2. Select "Start" - "Setting" - "Control Panel". The "Control Panel" dialog box opens.
3. Click the "System" icon. The "System Properties" dialog box opens.
4. Click "Network Identification".
5. Click the "Properties" button. The "Identification changes" dialog box opens.
6. Enter the name in the "Computer name" column.
7. Click the "OK" button.
8. Restart Windows 2000. Restart is necessary to enable the new settings.

Registering Group Names in the Central Monitor

Up to 16 group names can be registered for one network. If you do not divide instruments on a network into groups, registering group names is unnecessary. Registration can be done on the Name Registration window of the System Setup. Refer to Section 4 of the CNS-9701 operator's manual. This setting affects the entire network because group names are shared in the entire network.

Assigning a Group Name

Assign a group name to the central monitor, beds on the multiple patient receiver and bedside monitors on the network, respectively. The factory default setting group name for each instrument is “General”. If you do not divide instruments on a network into groups, assigning a group name is not necessary.

Central monitor:

Set the group name on the Name Registration window of the System Setup on the central monitor. Refer to the CNS-9701 operator’s manual.

Beds via the ORG-9200 multiple patient receiver:

Set the group name on the ORG Setting window of the System Setup on the central monitor. Refer to the CNS-9701 operator’s manual.

Bedside monitors:

Assign the group name to bedside monitors on the SYSTEM SETUP screen on each bedside monitor. Refer to the bedside monitor operator’s manual.

When the group name does not appear on the SYSTEM SETUP screen on the bedside monitors:

1. Turn off then turn on the bedside monitor.

2. Wait for 30 seconds and display the SYSTEM SETUP screen. The group name appears on the screen.

Checking the Bed Name and Group Name Setting

On the Monitor Setting window of the System Setup on the central monitor, you can check if the bed name and group name are properly assigned to each bed. Refer to the CNS-9701 operator’s manual.

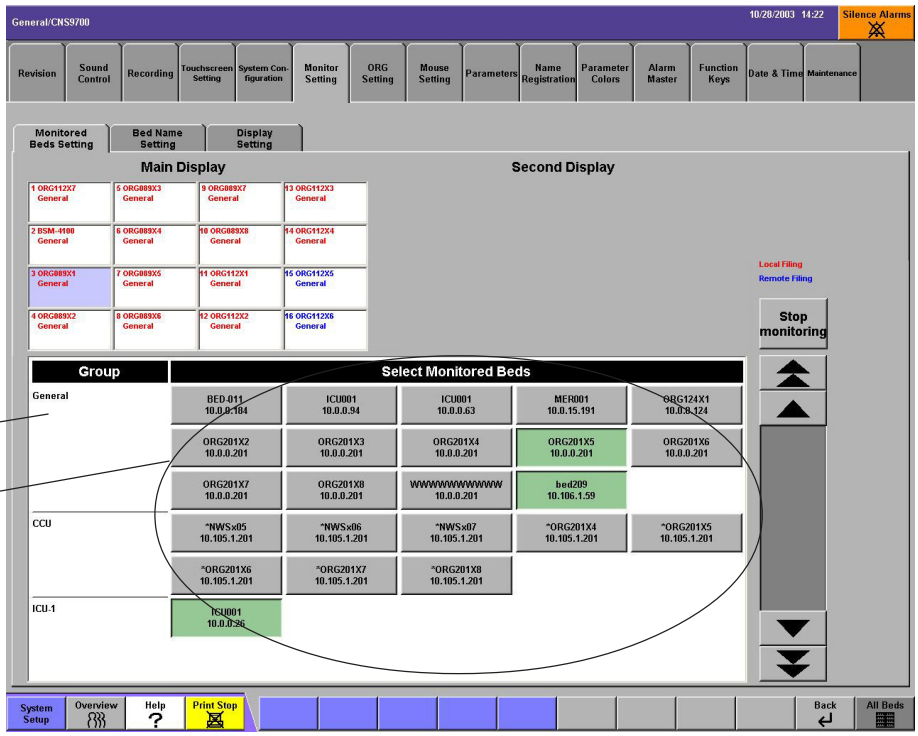

Selecting the Monitored Beds

One bedside monitor can be monitored on several central monitors, but the data can only be stored on one central monitor. When you register a monitored bed on the Monitor Settings of the System Setup, you will be asked if you want the central monitor to store the bed's data. Availability of setting and operations depends on whether or not the bed's data is saved in the central monitor or another central monitor. Refer to the CNS-9701 operator's manual.

A central monitor can monitor and store data of beds in a different group. However, it is recommended to monitor and store data of the beds in the same group as the central monitor so that data will not be mixed or lost.

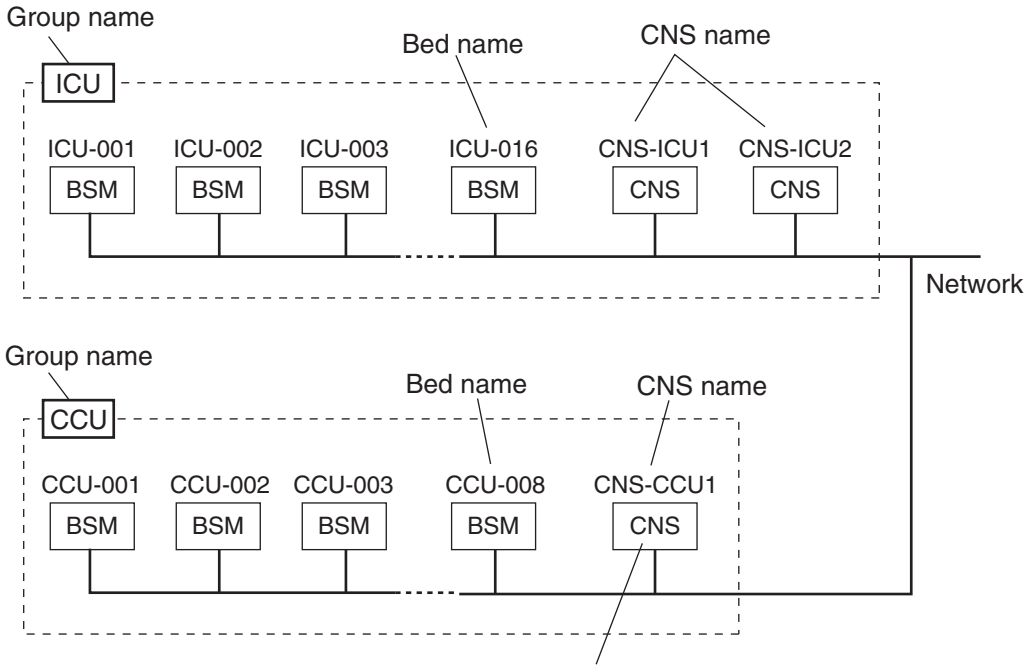

The CCU central monitor can monitor and store data of the beds in the ICU group. However, it is recommended to monitor and store data of the CCU beds in the CCU group so that data will not be lost.

CAUTION

The data of a bedside monitor cannot be stored on more than one central monitor. If the data of the same bedside monitor is stored on two central monitors, data communication cannot be properly performed or the data may be lost. Make sure that the bedside monitor data is saved only on one central monitor.

NOTE

For a 8000 series bed whose data is stored in a CNS-9301/9302 central monitor, some waveforms cannot be displayed on the Individual Bed screen of the CNS-9701 central monitor while the same patient's Individual Bed screen is displayed on the CNS-9301/9302 central monitor.

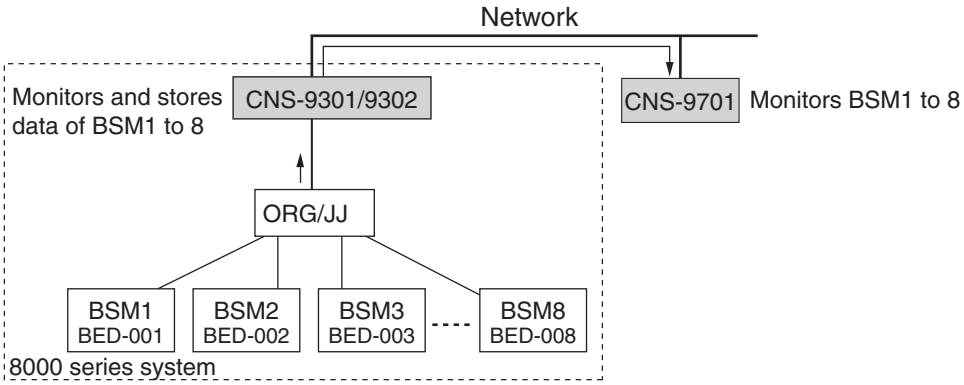

For 8000 series beds, refer to Section 1 "System Composition".

Changing Settings of System Setup, Patient Setting and Setup

Before using the central monitor, confirm that the settings on the System Setup window and the Patient Setting window are correct. Change them if necessary.

If you change the units, date and time when the network is in operation, the change on any instrument affects all instruments in the network.

Adding an Instrument to the Network During System Operation

An instrument can be connected to a network which is already running. The network does not need to be turned off. Check the following points.

- The network installation must comply with IEC 60601-1-1 “Safety Requirements for Medical Electrical Systems”. Refer to the Network and System installation guide and consult with a biomedical engineer or Nihon Kohden distributor.

- The IP address is correctly set on the instrument.

CAUTION

The network must be managed by the network administrator. Make sure that each monitor in the network has a different IP address. Otherwise, data communication cannot be performed properly and it causes incorrect monitoring. When adding a monitor to an already operating network, the IP address of the monitor must be set before connecting the monitor to the network.

- The power of the instrument to be added is turned off before connecting it to the network. When the instrument is properly connected to the network, turn the instrument power on.

- Assign the instrument name (bed name/CNS name) and group name to the instrument .

CAUTION

When the monitor is connected to a central network, set the bed name/ CNS name and group name on the monitor to correctly identify the bed on the central monitor. Otherwise the monitor cannot be managed properly. A new instrument is connected to the network with the factory default bed name/CNS name and group name. Therefore, if you don’t assign a proper name to the instrument after connection, it can cause patients to be mixed up.

- Check that the date and time and unit setting is the same as the other instruments in the network.

Section 9 Connector Pin Assignment

Sockets at the Rear of the Main Unit 9.1
- SOUND Socket 9.1
- TOUCH1/TOUCH2 Socket 9.1
- VIDEO1/VIDEO2 Socket 9.2
- RECORDER Socket 9.2
- PROTECT KEY Socket 9.2

This page is intentionally left blank.

Sockets at the Rear of the Main Unit

CAUTION

Connect only the specified instruments to the connector or sockets marked with ⚠ by following the specified procedure. Otherwise, electrical leakage current may harm the patient and operator.

SOUND Socket

Pin No.	Signal
1	L-Speaker
2	R-Speaker
3	GND

Central monitor main unit (MU-971RA/RJ/RK)
Stereo mini jack for 3-polar plug

LCD unit (VL-971R/RK)
Stereo mini jack for 3-polar plug

TOUCH1/TOUCH2 Socket

Male



Pin No.	Signal
1	Data Carrier Detect
2	Transmit Data
3	Receive Data
4	Data Set Ready
5	Ground
6	Data Terminal Ready
7	Clear To Send
8	Request To Send
9	Ring indicator
Case	Shield

Female



Central monitor main unit (MU-971RA/RJ/RK)
D-SUB 9 pin (male)

LCD unit (VL-971R/RK)
TOUCH SCREEN socket, D-SUB 9 pin (female)

VIDEO1/VIDEO2 Socket



Signal	Pin No.		Signal
RED	1	9	NC
GREEN	2	10	GND
BLUE	3	11	NC
NC	4	12	NC
GND	5	13	H-Sync
RED-GND	6	14	V-Sync
GREEN-GND	7	15	NC
BLUE-GND	8		
---	Case		Shield

Central monitor main unit (MU-971RA/RJ/RK)
D-SUB 15 pin (female)

LCD unit (VL-971R/RK)
VIDEO socket, D-SUB 15 pin (female)

RECORDER Socket

Male



Pin No.	Signal
1	Data Carrier Detect
2	Transmit Data
3	Receive Data
4	Data Set Ready
5	Ground
6	Data Terminal Ready
7	Clear To Send
8	Request To Send
9	Ring indicator
Case	Shield

Central monitor main unit (MU-971RA/RJ/RK)
D-SUB 9 pin (male)

Recorder unit (WS-971R)
PC socket, D-SUB 9 pin (male)

PROTECT KEY Socket

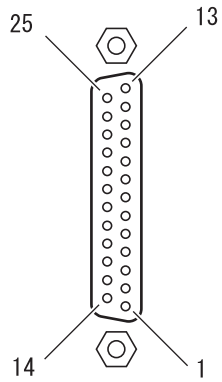

Signal	Pin No.		Signal
DATA0	1	14	READ
DATA1	2	15	RDRDY
DATA2	3	16	SYNC
DATA3	4	17	RDBK0
DATA4	5	18	ADDR0
DATA5	6	19	ADDR1
DATA6	7	20	ADDR2
DATA7	8	21	ADDR3
GND	9	22	ADDR4
WRITE	10	23	RDBK1
WRRDY	11	24	GND
ERROR	12	25	GND
RESET	13		

Central monitor main unit (MU-971RA/RJ/RK)
D-SUB 25 pin (female)